

User's Guide | LWA 7600

Class 1 Laser Product
Appareil Laser Classe 1
Laser Produkt Klass 1
IEC60825-1, 2014

Instrument	Wavelength	Max Power Emitted
7601-C	1515 nm – 1570 nm	< 5 mW
7601-CL	1520 nm – 1630 nm	< 5 mW
7601-O	1260 nm – 1360 nm	< 5 mW



Many regions prohibit the disposal of WEEE (Waste Electrical and Electronic Equipment) in the normal waste stream, to comply with the Restriction of Hazardous Substances (RoHS) released into the environment. Please contact your local waste authority for instructions on proper recycling of the electronic product(s) described in this *User Guide*.

User's Guide *LUNA LWA 7600*
© 2026

Luna Innovations Inc.
2270 Kraft Drive
Blacksburg, VA 24060
Phone: (866) 586-2682
Fax: (540) 961-5191
Support: support.lunainc.com
Web: www.lunainc.com

Table of Contents

1 Safety 1
2 Technical Support 2
3 Overview and Setup 3
3.1 Instrument Status Indicators 3
3.2 USB Connection 4
4 User Interface 4
4.1 UI Layout Overview 4
4.1.1 Status 5
4.1.2 Measure 5
4.1.3 Trace Settings 5
4.1.4 Turn Spectral Plot Display On/Off 9
4.1.5 Turn Event Table Display On/Off 9
4.2 Delay Plot 9
4.2.1 Plot Navigation 11
4.2.2 Single Cursor 11
4.2.3 Vertical Cursors 12
4.2.4 Horizontal Cursors 13
4.3 Spectral Plot 13
4.3.1 Spectral Plot Overview 13
4.3.2 Spectral Cursor 14
4.3.3 Operations on Spectral Plot 14
4.3.4 Cursors on the Spectral Plot 15
4.4 Event Table 16
4.4.1 Event Markers in the Delay Plot 17
4.4.2 Event Distances 17
4.5 Menu 19
4.5.1 Overview 19
4.5.2 File Operations 20
4.5.2.1 File Dialog 20
4.5.2.2 Open 22

4.5.2.3 Save 22
4.5.3 Settings 24
4.5.3.1 Acquisition Settings 24
4.5.3.2 Measurement Settings 25
4.5.3.3 Calibration Settings 26
4.5.3.4 Use Laser as Light Source 27
4.5.4 Configuration 27
4.5.4.1 Load Configuration 28
4.5.4.2 Save Configuration 28
4.5.4.3 Default Configuration 29
4.5.4.4 Delete Configuration 29
4.5.5 Help 30
4.5.5.1 Documentation 30
4.5.5.2 Update Feature Keys 30
4.5.5.3 About 30
4.6 Remote User Interface 32
4.6.1 Installation 32
4.6.2 Disconnected Mode 32
4.6.3 Remote Connection 33
5 SCPI Interface 36
5.1 Introduction to SCPI 36
5.2 Luna LWA 7600 SCPI Instrument Model 36
5.3 SCPI is Not a Data Streaming Protocol 36
5.4 Example SCPI Command Sequences 37
5.4.1 Example 1: Take Sequential Measurements 37
5.4.2 Example 2: Get Multiple Results from a Single Measurement 38
5.4.3 Example 3: Get a Subset of the Measurement Data 38
5.5 SCPI Command Reference 39
5.5.1 SENSe Subsystem 39
5.5.1.1 [:SENSe][:IFO]:DELay 39
5.5.1.2 [:SENSe][:IFO]:DELay? 39
5.5.1.3 [:SENSe][:IFO]:LENGth 39

5.5.1.4 [:SENSe][:IFO]:LENGth? 40
5.5.1.5 [:SENSe][:IFO]:GINDex 40
5.5.1.6 [:SENSe][:IFO]:GINDex? 40
5.5.1.7 [:SENSe][:IFO]:FOCUs 40
5.5.1.8 [:SENSe][:IFO]:FOCUs? 41
5.5.1.9 :SENSe:WAVelength:SPAN 41
5.5.1.10 :SENSe:WAVelength:SPAN? 41
5.5.1.11 :SENSe:WAVelength:CENTer 41
5.5.1.12 :SENSe:WAVelength:CENTer? 42
5.5.1.13 :SENSe:WAVelength:STARt? 42
5.5.1.14 :SENSe:WAVelength:STOP? 42
5.5.2 SOURce Subsystem 42
5.5.2.1 :SOURce:WAVelength 42
5.5.2.2 :SOURce:WAVelength? 43
5.5.3 OUTPut Subsystem 43
5.5.3.1 :OUTPut[:STATe] 43
5.5.3.2 :OUTPut[:STATe]? 43
5.5.4 CALCulate Subsystem 43
5.5.4.1 :OFDR:FILTer:GAUSsian[:STATe] 43
5.5.4.2 :OFDR:FILTer:GAUSsian[:STATe]? 44
5.5.4.3 :OFDR:FILTer:GAUSsian:WIDTh 44
5.5.4.4 :OFDR:FILTer:GAUSsian:WIDTh? 44
5.5.5 Measurement Instructions 44
5.5.5.1 :CONFigure? 44
5.5.5.2 :CONFigure:RL 45
5.5.5.3 :CONFigure:RL? 45
5.5.5.4 :CONFigure:IL 45
5.5.5.5 :CONFigure:IL? 45
5.5.5.6 :CONFigure:OFDR 46
5.5.5.7 :CONFigure:OFDR? 46
5.5.5.8 :CONFigure:DISTance 46
5.5.5.9 :CONFigure:DISTance? 46

5.5.5.10 :CONFigure:SPECtral 46
5.5.5.11 :CONFigure:SPECtral? 47
5.5.5.12 :CONFigure:EVENt 47
5.5.5.13 :CONFigure:EVENt? 47
5.5.5.14 :BINary 48
5.5.5.15 :BINary? 48
5.5.5.16 :FORMat:DATA 48
5.5.5.17 :FORMat:DATA? 49
5.5.5.18 :FETCh? 49
5.5.5.19 :FETCh:RL? 49
5.5.5.20 :FETCh:IL? 49
5.5.5.21 :FETCh:OFDR? 49
5.5.5.22 :FETCh:DISTance? 50
5.5.5.23 :FETCh:SPECtral? 50
5.5.5.24 :FETCh:GD? 50
5.5.5.25 :FETCh:WAVelength? 51
5.5.5.26 :FETCh:EVENt? 51
5.5.5.27 :READ[:<function>]? 51
5.5.5.28 :MEASure[:<function>]? 52
5.5.6 TRIGger Subsystem 52
5.5.6.1 :INITiate[:ALL] 52
5.5.7 MMEMory Subsystem 52
5.5.7.1 :MMEMory:LOAD:STATe 52
5.5.7.2 :MMEMory:STORe:STATe 53
5.5.7.3 :MMEMory:STORe[:CUSTom] 53
5.5.8 SYSTem Subsystem 54
5.5.8.1 :SYSTem:ERRor[:NEXT]? 54
5.5.8.2 :SYSTem:VERSion? 54
5.5.9 STATus Subsystem 54
5.5.9.1 :STATus:OPERation:CONDition? 54
5.5.9.2 :STATus:OPERation[:EVENt]? 55
5.5.9.3 :STATus:OPERation:ENABle 56

5.5.9.4 :STATus:OPERation:ENABle? 56
5.5.9.5 :STATus:QUEStionable:CONDition? 56
5.5.9.6 :STATus:QUEStionable[:EVENt]? 57
5.5.9.7 :STATus:QUEStionable:ENABle 58
5.5.9.8 :STATus:QUEStionable:ENABle? 58
5.5.9.9 :STATus:PRESet 58
5.5.10 Common Commands and Queries 59
5.5.10.1 *STB? – Read Status Byte Query 59
5.5.10.2 *SRE -- Service Request Enable Command 60
5.5.10.3 *SRE? -- Service Request Enable Query 61
5.5.10.4 *ESR? -- Standard Event Status Register Query 61
5.5.10.5 *ESE -- Standard Event Status Enable Command 61
5.5.10.6 *ESE? -- Standard Event Status Enable Query 62
5.5.10.7 *WAI -- Wait-to-Continue Command 62
5.5.10.8 *OPC -- Operation Complete Command 62
5.5.10.9 *OPC? -- Operation Complete Query 63
5.5.10.10 *CLS -- Clear Status Command 63
5.5.10.11 *RST -- Reset Command 63
5.5.10.12 *IDN? -- Identification Query 64
5.5.10.13 *TST? -- Self-Test Query 64
5.5.10.14 *RCL – Recall Command 65
5.5.10.15 *SAV – Save Command 65
5.6 SCPI Error Codes 65
Appendix A Theory of Operation 67

1 Safety

The advisory words **Danger**, **Warning** and **Caution** used in this manual identify the level of hazard that may be encountered by the user.

- **DANGER** means if the danger is not avoided, it will cause death or serious injury.
- **WARNING** means if the warning is not heeded, it can cause death or serious injury.
- **CAUTION** means if the precaution is not taken, it may cause minor or moderate injury.

⚠ Warning

The protection provided by the equipment may be impaired if the equipment is used in a manner not specified by the manufacturer, resulting in serious injury or death.

The power cord is the main electrical disconnect for this equipment. If it is necessary to ensure no power to the unit, remove the power cord.

The use of controls, adjustments, performance, or procedures other than those specified herein may result in hazardous laser radiation exposure and one or more safety protections may be impaired or rendered ineffective.

⚠ Attention

La protection fournie par l'équipement peut être compromise si l'équipement est utilisé d'une manière non spécifiée par le fabricant, entraînant des blessures graves ou la mort.

Le cordon d'alimentation est le principal disjoncteur électrique de cet équipement. S'il est nécessaire de ne pas mettre l'appareil hors tension, retirez le cordon d'alimentation.

L'utilisation de commandes, d'ajustements, de performances ou de procédures autres que celles spécifiées ici peut entraîner une exposition dangereuse au rayonnement laser et une ou plusieurs protections de sécurité peuvent être altérées ou rendues inefficaces.

2 Technical Support

If you have concerns with or questions about the information contained in this document, contact our technical support staff at: support.lunainc.com

3 Overview and Setup

The Luna LWA 7600 is a fast and simple-to-use analyzer for passive optical components and modules. The Luna LWA 7600 extends the industry-leading optical frequency domain reflectometry (OFDR) platform from Luna Innovations to manufacturing test and quality control applications.

Unlike traditional passive component testers, the Luna LWA 7600 measures and analyzes the Insertion Loss (IL) and Return Loss (RL) distribution, as well as length, working in either reflection or transmission. The Luna LWA 7600 features extremely high sensitivity, 20 µm spatial sampling resolution, and very fast scanning for high test throughput.

This User's Guide covers how to set up and use the application software. Please refer to the Luna LWA 7600 Setup Guide for information regarding the proper methods of setting up and maintaining the hardware.

3.1 Instrument Status Indicators

The front panel of the LWA 7600 has two LED system status indicators as shown in Figure 3-1 (highlighted by the green box).

Power Lit while the system is powered on (press to turn on/off)
Reset Indicates instrument status

White	Blinking	Instrument Starting
White	Solid	Instrument Idle
Orange	Blinking	Laser is Starting
Orange	Solid	Laser Started
Blue	Blinking	System Arming
Blue	Solid	System Collecting Measurements
Purple	Blinking	Embedded SW Update in Progress
Red	Blinking	Embedded SW Update Failed



Figure 3-1 LWA 7600 Power and Reset Buttons, shown in green box.

3.2 USB Connection

The LWA 7600 must connect to the controller as a USB 3.0 device. If it connects as a USB 2.0 device instead, the user interface shows the message in Figure 3-2 and the status displays “Instrument enumerated as USB 2.0 - unplug the USB cable, flip the connector, and reconnect”. To fix it, unplug one end of the USB cable, turn the connector over, and plug it back in. If the problem persists, try a different USB port or cable.

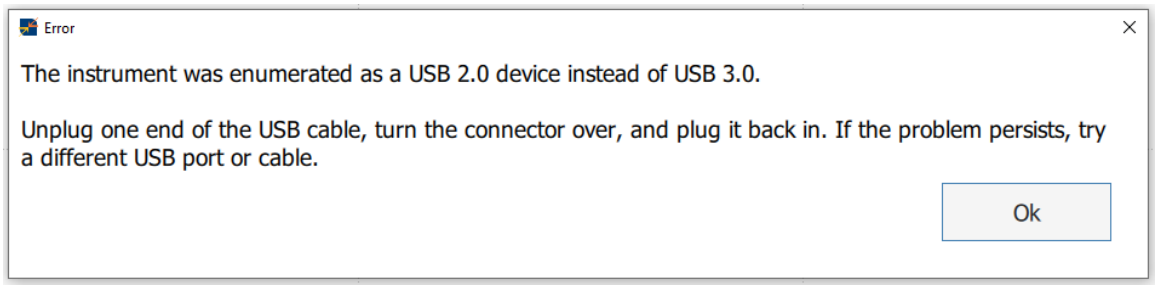


Figure 3-2 USB 2.0 Warning

4 User Interface

Let us take a tour of the application’s User Interface (UI). The tour will start with an introduction to the UI layout, then explains each UI component: the Delay Plot, Spectral Plot, Event Table, Measurement Controls and information displays.

The UI supports up to four traces being displayed at a time. The first trace is the data actively being measured. The other three traces can be copied from another trace or a loaded data file saved from an earlier session.

4.1 UI Layout Overview

After you power on the system and start the Luna LWA 7600 software on the controller PC, the application UI screen will appear on the PC screen. The system will initialize, then launch the hardware in reflection mode and display one measurement result on the screen. Figure 4-1 is an illustration of a typical UI screen layout with all optional displays turned on for a reflection measurement (for a transmission measurement, the layout is the same except that the elements related to return loss are omitted).

The upper section of UI screen is for the display of Measurement Controls.

The lower section of UI screen is the Delay Plot (upper left side) along with an optional Spectral Plot (lower left side) and an optional Event Table (right side). The Delay Plot would be scaled to take up the whole lower section area if the optional displays are turned off (which is the default when the system is just powered up).

Each of the above UI components is further explained in the following titled sections, respectively.

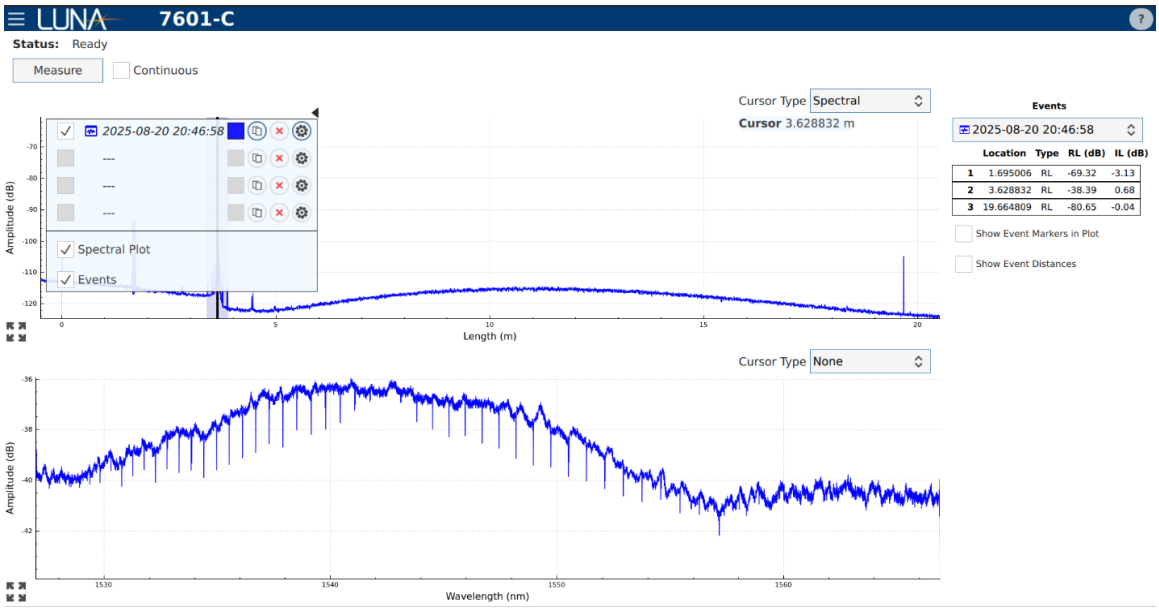


Figure 4-1 Screen Layout

4.1.1 Status

The system Status is indicated in the top left corner of the user interface. The status displays the current state of the system including messages regarding system startup, ready state, measuring state, and error states.

4.1.2 Measure

On startup, the user interface will display the latest measurement. Click the Measure button Measure to perform a new single measurement. Check the Continuous checkbox to perform continuous measurements. Click the Measure button to start the continuous measurement. This will change the Measure button to display “Stop” Stop Continuous. Click the Stop button to stop the measurements.

4.1.3 Trace Settings

The UI supports up to four traces to be displayed at a given time as shown in Figure 4-2. Click the left arrow ◀ at the upper right of the Trace Legend to minimize the legend. To restore the Trace Legend, click the right arrow next to the y-axis of the plot ▶.

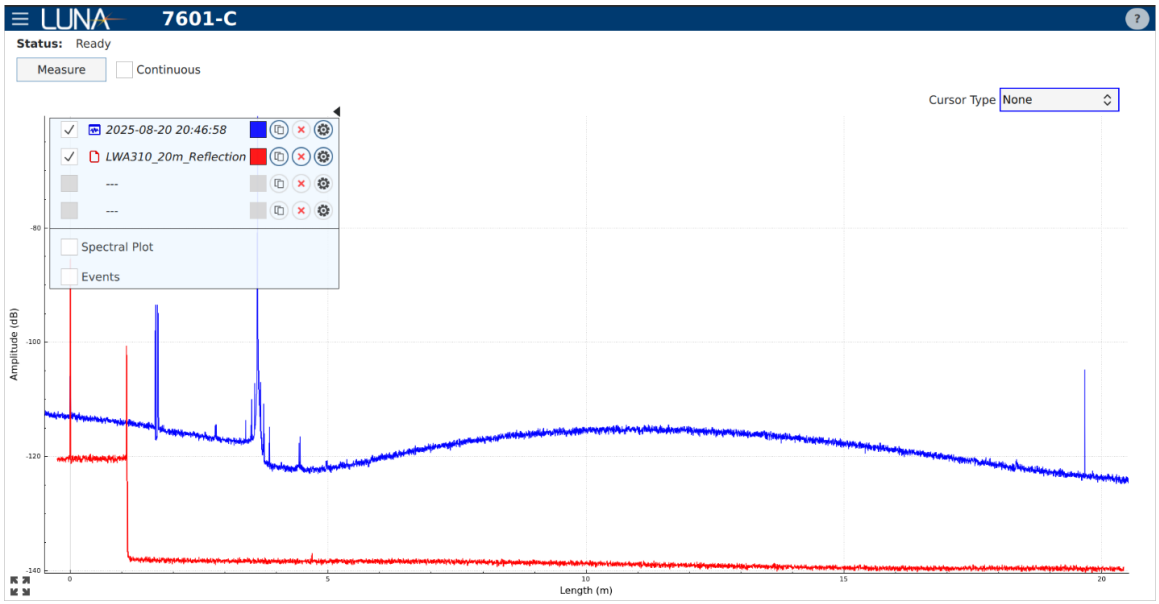


Figure 4-2 Multiple Traces

The first trace is the current measurement . The other three traces can be a loaded OFDR file or a copy of another trace . The Trace Legend as shown in Figure 4-3, allows the user to control the aspects of the traces. Each trace has a checkbox to display or not display that specific trace.

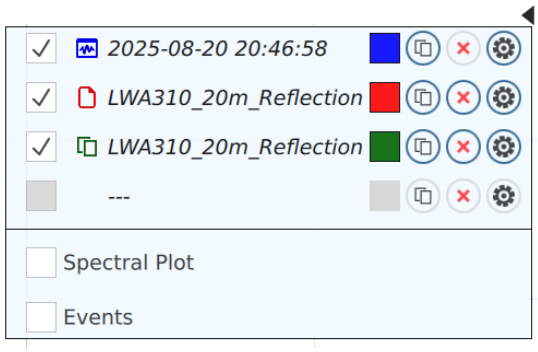


Figure 4-3 Trace Legend

Click the Color Square to change the color of that trace. This will bring up a color dialog as shown in Figure 4-4. The associated icon will also change to the selected color for easier reference.



Figure 4-4 Color Dialog

The selected trace color is saved on the computer running the user interface and is kept when the user interface is restarted. Right-click the Color Square or press and hold it to show the reset options as shown in Figure 4-5. Select Reset to default color Reset to default color to return that trace to its default color, or select Reset all colors to default Reset all colors to default to return all traces to their default colors.

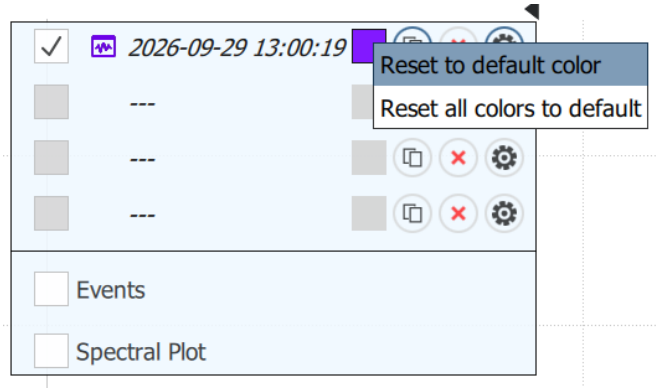


Figure 4-5 Reset Options

Click the Copy Trace button to copy that trace into the first empty trace. Click the Clear Trace button to clear a loaded or copied trace, for example to free a trace when all four are in use or when a trace is no longer needed. The measured trace cannot be cleared.

Hover over the Gear button to display settings related to the associated trace as shown in Figure 4-6.

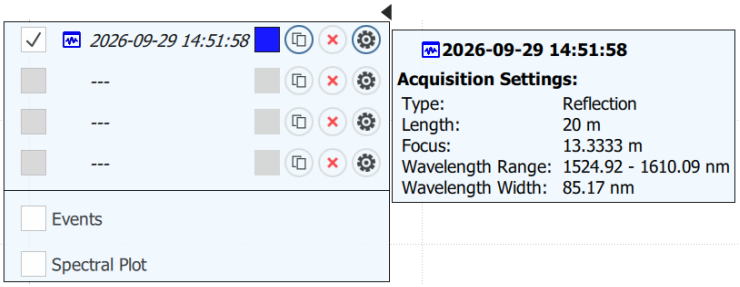


Figure 4-6 Acquisition Settings

Click the Gear button to open the Trace Settings dialog as shown in Figure 4-7. This dialog provides the operating settings for the trace and allows the user to change certain data parameters.

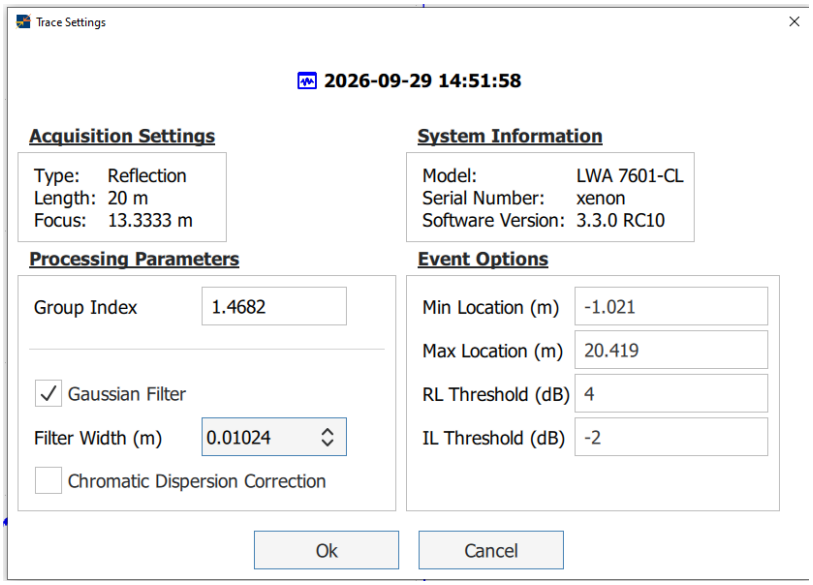


Figure 4-7 Trace Settings

The **Acquisition Settings** and **System Information** sections show how the trace was measured: its acquisition type, length and focus, and the model, serial number and software version of the system that measured it. For a trace loaded from a file, these are the values saved in the file. To change the acquisition settings for new measurements, see section “4.5.3.1 Acquisition Settings”.

Processing Parameters



- *Group Index* – allows the user to specify the group index of refraction (range: 1 – 4).
- *Gaussian Filter* – if checked, a Gaussian filter is applied to the data to smooth out the graph. This is turned on by default.

- *Filter Width* – sets the Gaussian Filter width in display units which is meters by default, options are 0.00016 m, 0.00032 m, 0.00064 m, 0.00128 m, 0.00256 m, 0.00512 m and 0.01024 m (default).
- *Chromatic Dispersion Correction* – if checked, each event that chromatic dispersion has spread into a broad peak is restored to a sharp reflection. This is turned off by default.


Event Options

- *Min Location* and *Max Location* – allows the user to specify the length/location range of events reported in the Event Table.
- *RL Threshold* and *IL Threshold* – set the minimum RL or IL an event must have to be reported in the Event Table.

4.1.4 Turn Spectral Plot Display On/Off

Check the Spectral Plot checkbox  to display the Spectral Plot. The Spectral Plot is not displayed by default after you first open the application. When the Spectral Plot checkbox is checked, the Cursor Type  will change to Spectral automatically. Uncheck the Spectral Plot checkbox to hide the Spectral Plot and return the Cursor Type to None. See section "4.3 Spectral Plot" for more information.

4.1.5 Turn Event Table Display On/Off

Check the Events checkbox  to display the Event Table. The Event Table is not displayed by default after you first open the application. Uncheck the Events checkbox to hide the Event Table. See section "4.4 Event Table" for more information.

4.2 Delay Plot

When you first open the application, the UI screen appears with the Delay Plot as shown in Figure 4-8. The Delay Plot screen displays acquired measurements in the Time Delay Domain (reflection amplitude vs time of flight, or reflection amplitude vs length).

The plot x-axis unit can be displayed in one of the following five options: m, mm, in, ft or ns.


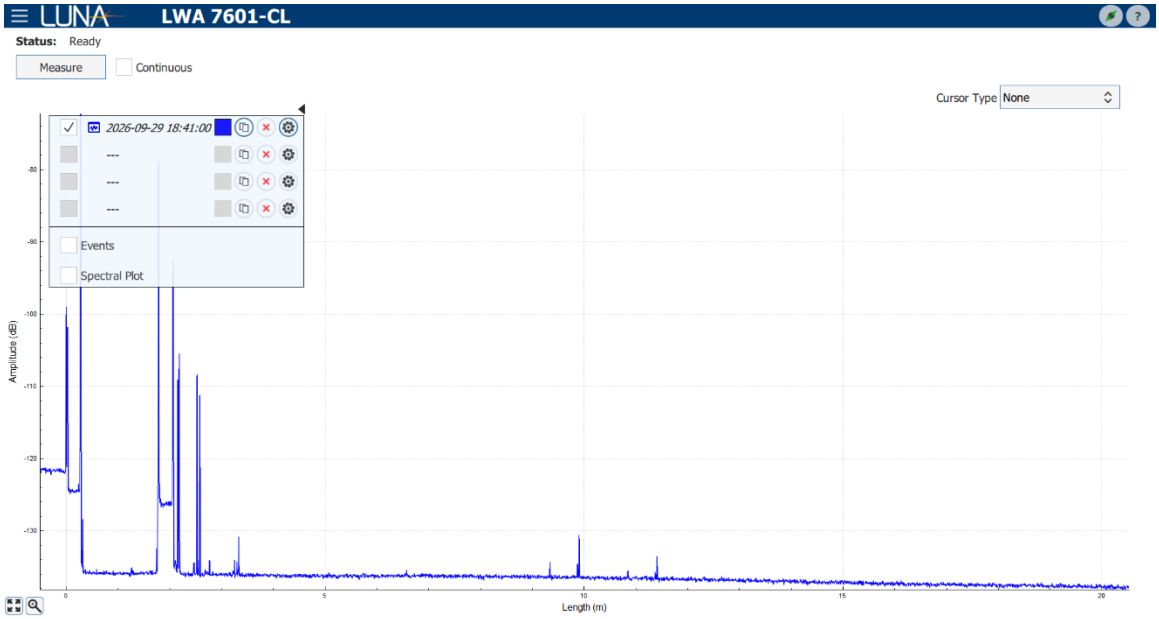


Figure 4-8 Delay Plot

The Delay Plot Screen allows the user to change the Cursor Type to one of the following values by choosing a Cursor Type selection in the upper right area of the plot:



- None – Only the graph of the acquired data is displayed.
- Single – A single vertical cursor is shown that allows for RL and IL measurements to be made.
- Vertical – Two vertical cursors are shown that can be used to make length measurements.
- Horizontal – Two horizontal cursors are shown that can be used to make IL measurements and compare the reflectivity of various features in the measurement.
- Spectral – A single vertical cursor selects the data shown in the Spectral Plot; it is only available when the Spectral Plot checkbox is checked (see section “Spectral Cursor Spectral Cursor”).

Cursors can be moved by dragging them across the screen by using a mouse. When the cursors are selected and are being moved, they will change color to black (The cursor turns black when you

press it, indicating that it can be moved). Clicking once on the cursor will cause it to snap to the highest point within its highlighted zone.

4.2.1 Plot Navigation

The plots shown in the Luna LWA 7600 user interface can all be manipulated through mouse or touchpad actions on the laptop PC.

Panning – The plot can be panned over the X and Y axes by pressing and dragging at any point within the plot.

Zooming – The plot can be zoomed using a two-finger pinch or expanding motion at any point within the plot on touchpad or scrolling wheel on a mouse.

Constrained Panning or Zoom – It is possible to constrain the panning and zooming to one of the two axes by first left clicking on the desired axis. It will turn blue while panning and zooming is constrained. While an axis is selected, its minimum and maximum values are shown at the ends of the axis. Click either value to type a new value, and press Enter to apply it, as shown in Figure 4-9.

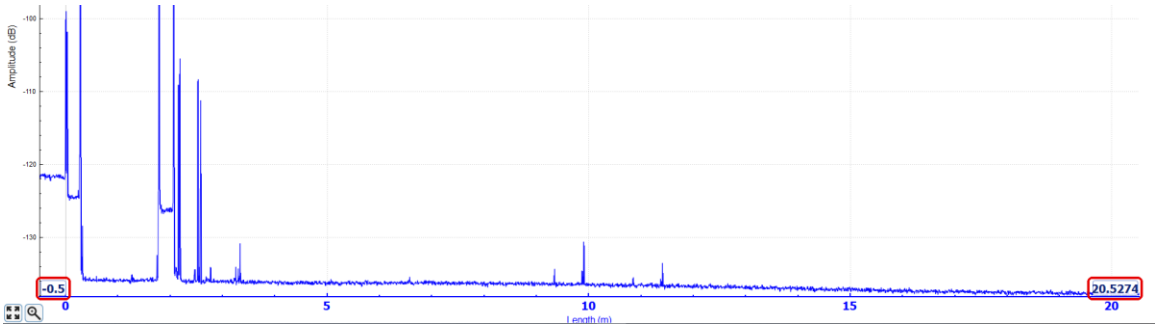


Figure 4-9 Editing an Axis Limit

Plot Rescaling – Double-click an axis to scale it to fit all data in the range.

Rescale Plot – Click on the Rescale Plot button on the lower left of the plot to rescale the entire plot to fit the window.

Zoom to Box – Click on the Zoom to Box button to turn on box zoom, then drag a box around the area to zoom into. Box zoom turns off automatically after the zoom. To turn it off without zooming, click the button again.

4.2.2 Single Cursor

The single cursor view provides a single vertical cursor with integration regions for measurement of both the RL and IL across an event as shown in Figure 4-10. The region with red shadowing is integrated to provide an RL measurement. The two regions with grey shadowing are used to compute the IL. The corresponding RL Width and IL Width can be changed in Measurement Settings. See section “4.5.3.2 Measurement Settings.” Data will be displayed in the upper right for all visible traces.

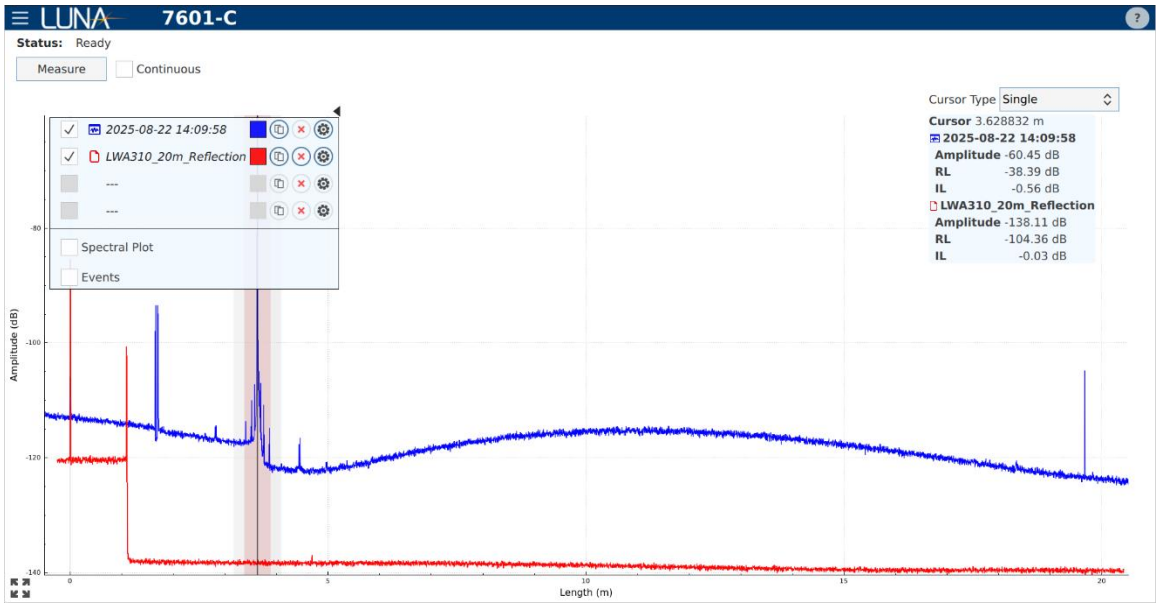


Figure 4-10 Single Cursor View

4.2.3 Vertical Cursors

The vertical cursor view provides two cursors that can be used to measure the length between two events or measure the IL over any distance as shown in Figure 4-11. The RL, position, and IL information is shown in the upper right area of the plot, under the Cursor Type selection. Data is shown for any visible trace.

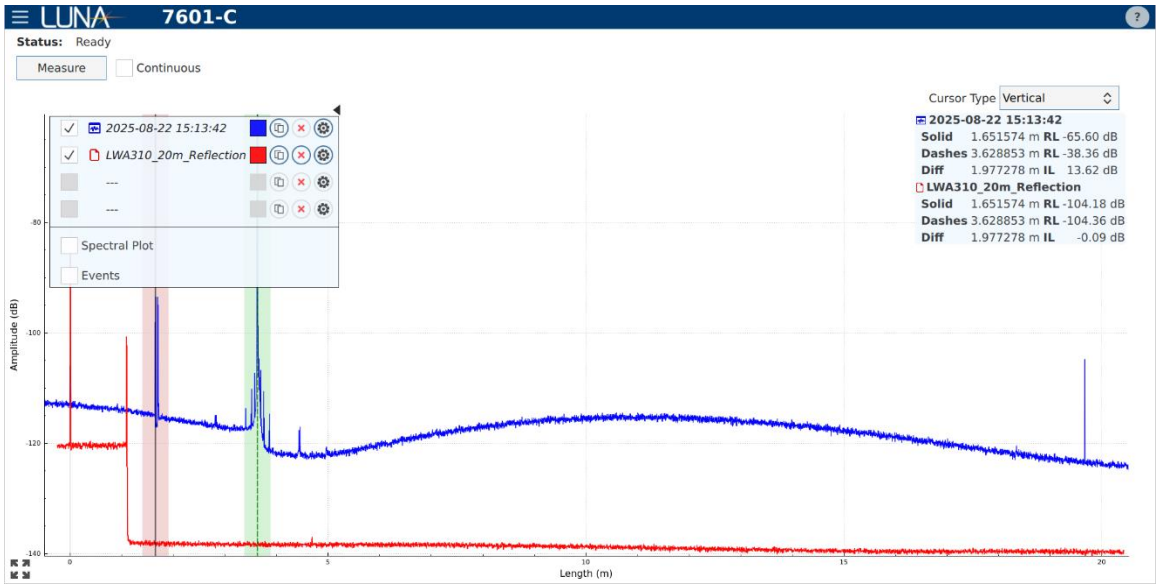


Figure 4-11 Vertical Cursor View

4.2.4 Horizontal Cursors

The horizontal cursors are used to compare the amplitude of two events in the data as shown in Figure 4-12.

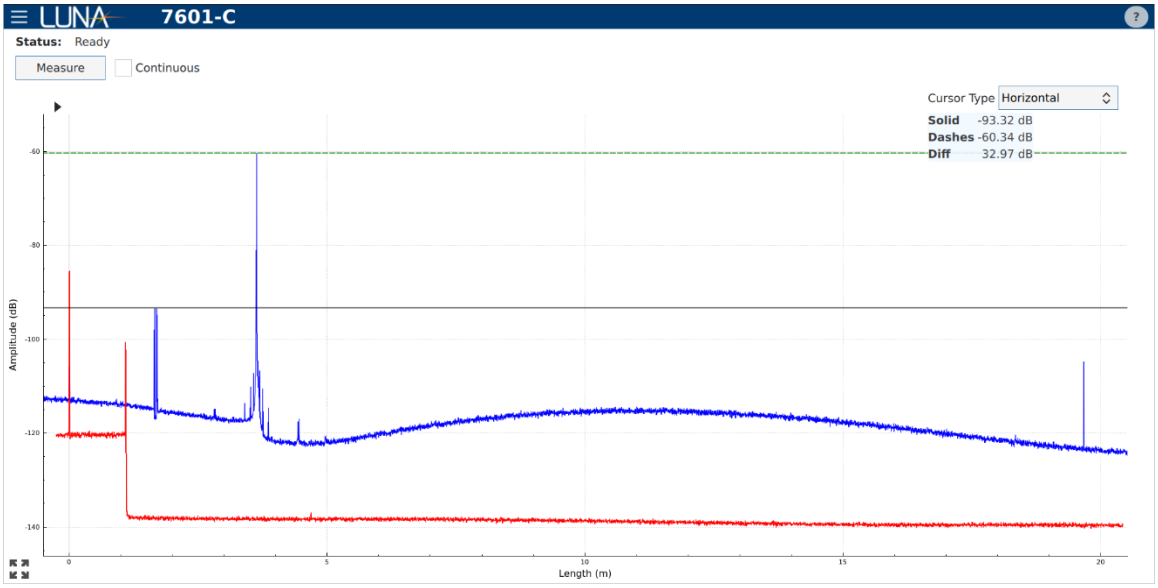


Figure 4-12 Horizontal Cursor View

It is important to remember that the amplitude data can be shown with varying levels of filtering which may make reflection peaks look smaller than they truly are.

4.3 Spectral Plot

4.3.1 Spectral Plot Overview

Check the Spectral Plot checkbox ☑ Spectral Plot in the plot legend to show the Spectral Plot. A single vertical Spectral Cursor is displayed in the upper Delay Plot. The calculated Spectral Loss and/or Group Delay of the given set of data (defined by the Spectral Cursor) is displayed as a function of optical wavelength in the lower Spectral Plot as shown in Figure 4-13.

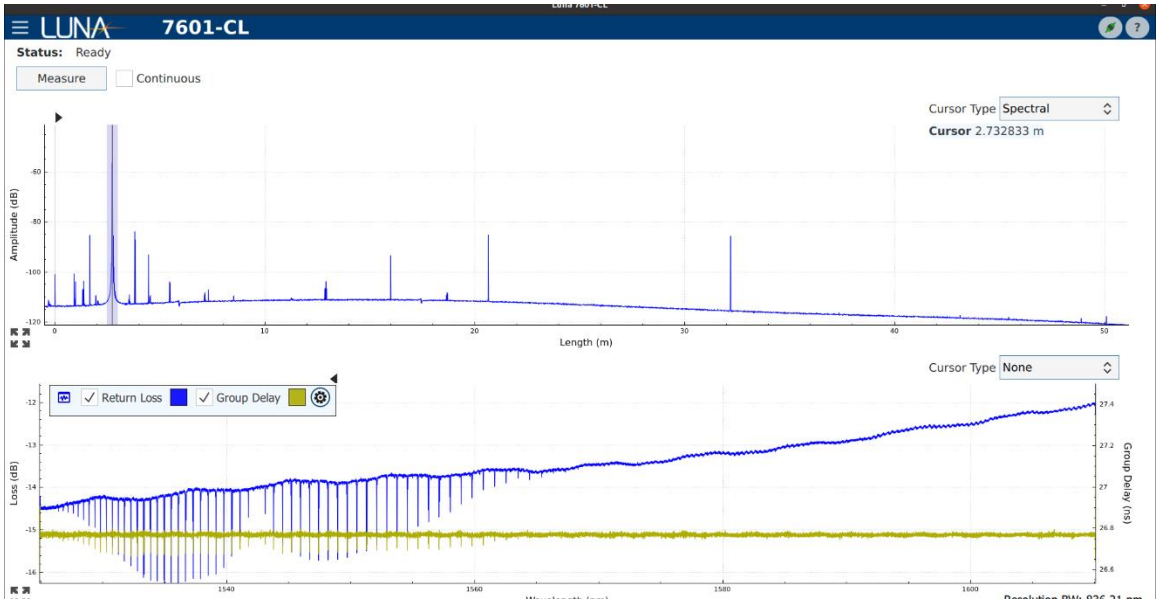


Figure 4-13 Spectral Plot

4.3.2 Spectral Cursor

The cursor is only available for selection when the Spectral Plot checkbox is checked. The single vertical cursor is used to select a windowed range in the Delay Plot and view a calculated metric (e.g., return loss, group delay) in the Spectral Plot.

4.3.3 Operations on Spectral Plot


Manipulating the Spectral Cursor selects the range of Time Delay Domain data used to compute the spectral loss and group delay. The location of the Spectral Cursor data selection range in the Delay Plot can be changed by moving the cursor to different locations in the plot. The width of the data selection range can be changed with the Spectral Cursor Width setting as described in section “4.5.3.2 Measurement Settings”.

The Resolution BW in the lower right of the Spectral Plot is the spectral resolution, set by the Spectral Cursor width 

.

The wavelength axis of the Spectral Plot covers the wavelength range the trace was acquired with, set in Acquisition Settings (see “4.5.3.1 Acquisition Settings”).

As in the Delay Plot, you can use cursors to analyze the Spectral Plot data. The application allows the user to change the Cursor Type of the Spectral Plot to one of three possible values:

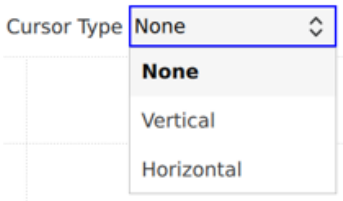

- None – Only the graph of the acquired data is displayed, no characteristics of the data are shown.
- Vertical – using two vertical cursors, displays the location at each cursor and the difference between them.
- Horizontal – using two horizontal cursors, displays the amplitude at each cursor location along with the difference between them.

Click the Color Square next to Return Loss (Insertion Loss for transmission traces) or Group Delay to change the color of that trace. This will bring up a color dialog as shown in Figure 4-4.

These colors are saved and can be reset the same way as trace colors as described in section "4.1.3 Trace Settings".

Click the Gear button  next to a trace in the Spectral Plot legend to open the Spectral Settings dialog for that trace, as shown in Figure 4-14.

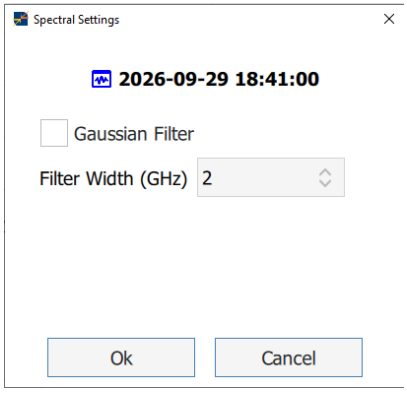


Figure 4-14 Spectral Settings

- *Gaussian Filter* – if checked, a Gaussian filter is applied to smooth both the loss and the Group Delay curves of the trace. This is turned off by default.
- *Filter Width* – sets the Gaussian Filter width in GHz, options are 0.5, 1, 2 (default), 5, 10 and 20 GHz.

4.3.4 Cursors on the Spectral Plot

When using Vertical or Horizontal cursors on the Spectral Plot, the values shown in the cursor readout depend on which traces are enabled by the Return Loss and Group Delay checkboxes in the spectral plot legend.

Vertical Cursors - Two vertical cursors (Solid and Dashes) are placed on the Spectral Plot as shown in Figure 4-15. For each cursor, the readout shows the wavelength, the corresponding Return Loss (when Return Loss is checked), and the corresponding Group Delay (when Group Delay is checked). The Diff value is the wavelength difference between the two cursors, and the IL value is the Insertion Loss between the cursor locations. For a transmission trace, the readout shows the Insertion Loss at each cursor instead of the Return Loss, and there is no IL value between the cursors.

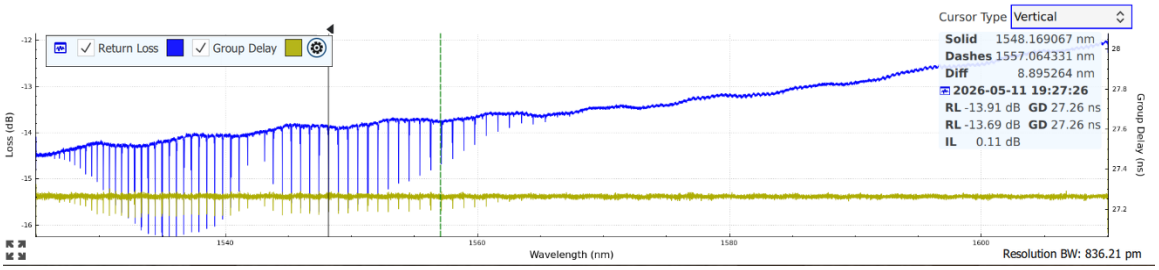


Figure 4-15 Vertical Cursors on Spectral Plot

Horizontal Cursors - Two horizontal cursors (Solid and Dashes) are placed on the Spectral Plot. The readout shows the y-axis value at each cursor and the difference (Diff) between them.

4.4 Event Table

The Event Table lists the return loss (RL) and insertion loss (IL) events detected in a trace, as shown in Figure 4-16. The events listed are those above the RL and IL thresholds and between the Min and Max Locations set in the trace's Event Options (see "4.1.3 Trace Settings").

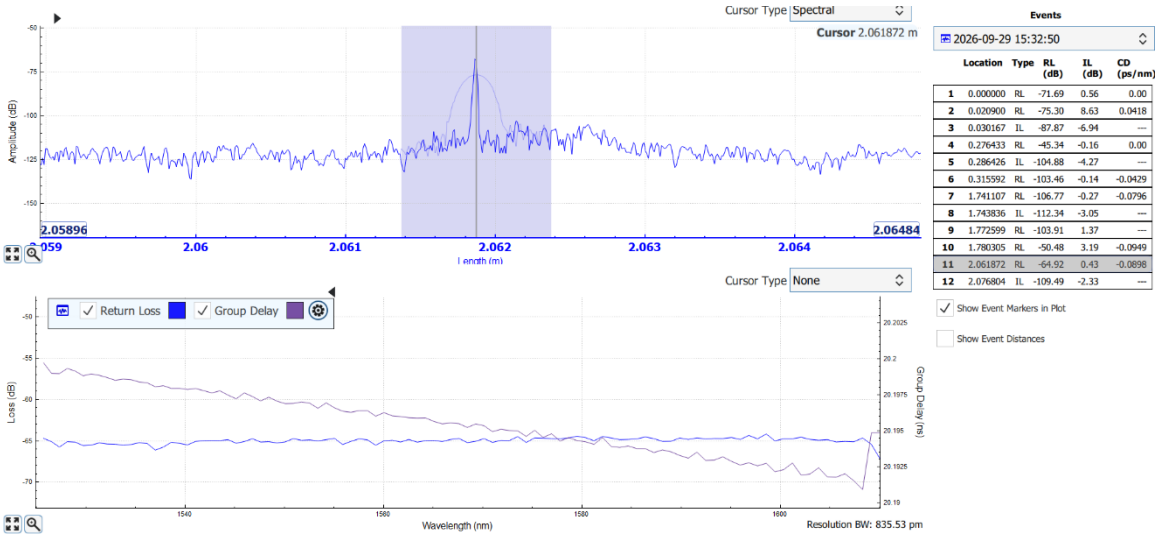


Figure 4-16 Event Table

For each event, the table shows its location, its type (RL or IL), and its return loss and insertion loss. For a transmission measurement, only insertion loss is shown. When Chromatic Dispersion

Correction is turned on for the trace, a CD (ps/nm) column shows the dispersion measured at each event; --- means no dispersion value could be measured for the event.

The drop-down list above the Event Table allows for choosing between the different traces as shown in Figure 4-17.

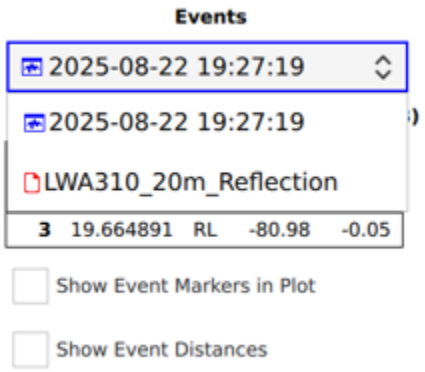


Figure 4-17 Event Table Trace List

4.4.1 Event Markers in the Delay Plot

You can check/enable the “Show Event Markers in Plot” checkbox to show vertical markers on all event locations as shown in Figure 4-18.

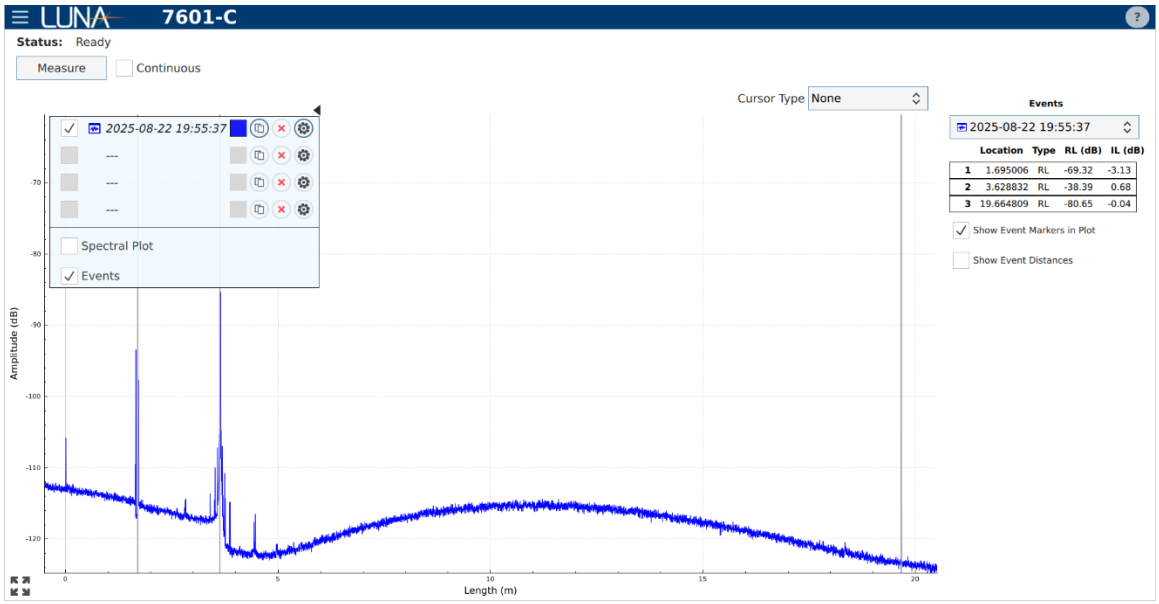


Figure 4-18 Show Event Markers in Plot

4.4.2 Event Distances

You can check/enable the "*Show Event Distances*" checkbox to show relative distances from the first event as shown in Figure 4-19.

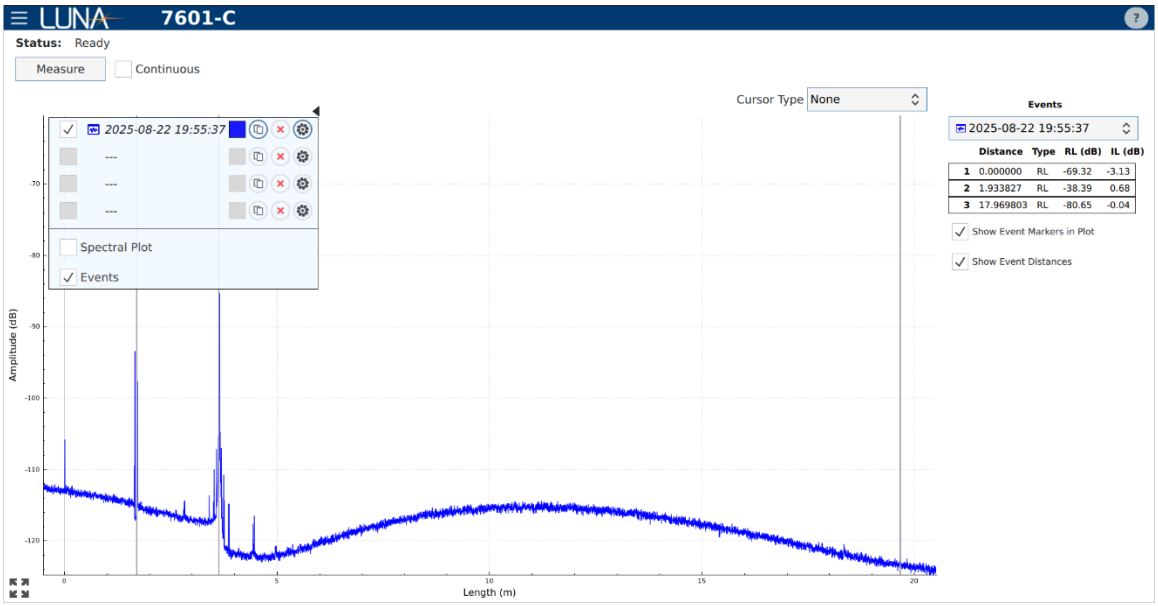


Figure 4-19 Show Event Distances

With the Cursor Type set to None or Horizontal, clicking an individual event draws a marker at that event location and highlights the event that is selected as shown in Figure 4-20. The distances are updated relative to the event that was selected. Clicking the event again removes the marker. With the Single or Spectral cursor, clicking an event moves that cursor to the event location instead; with the Vertical cursors, the closer of the two cursors moves.

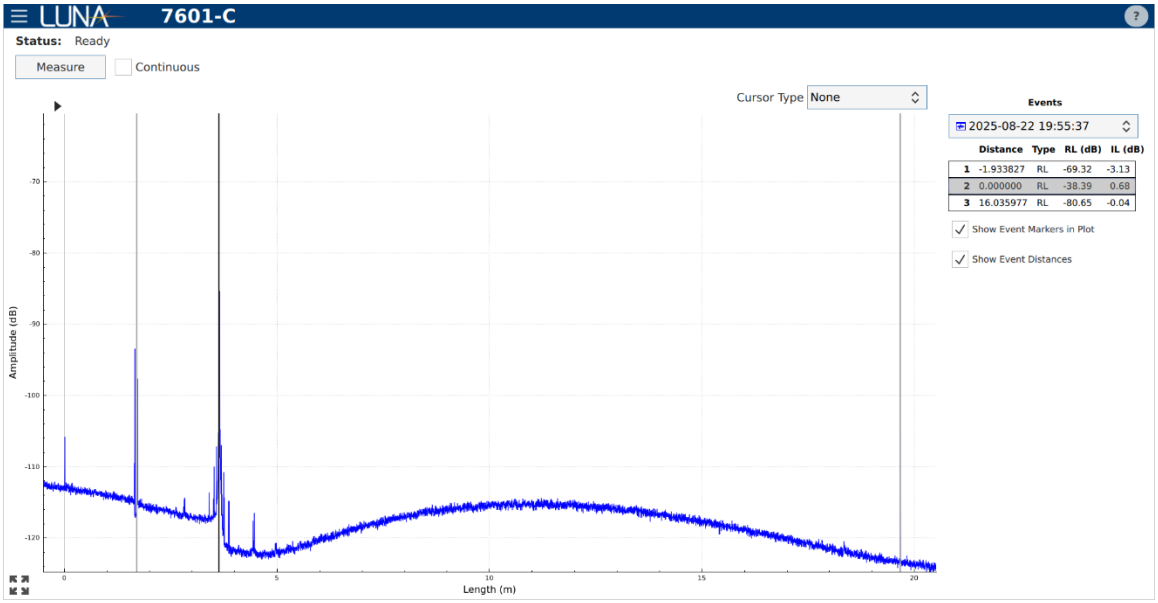


Figure 4-20 Clicking an event

Double-clicking an entry in the Event Table zooms the plot to that event's location as shown in Figure 4-21. In the example, event 2 was double-clicked.

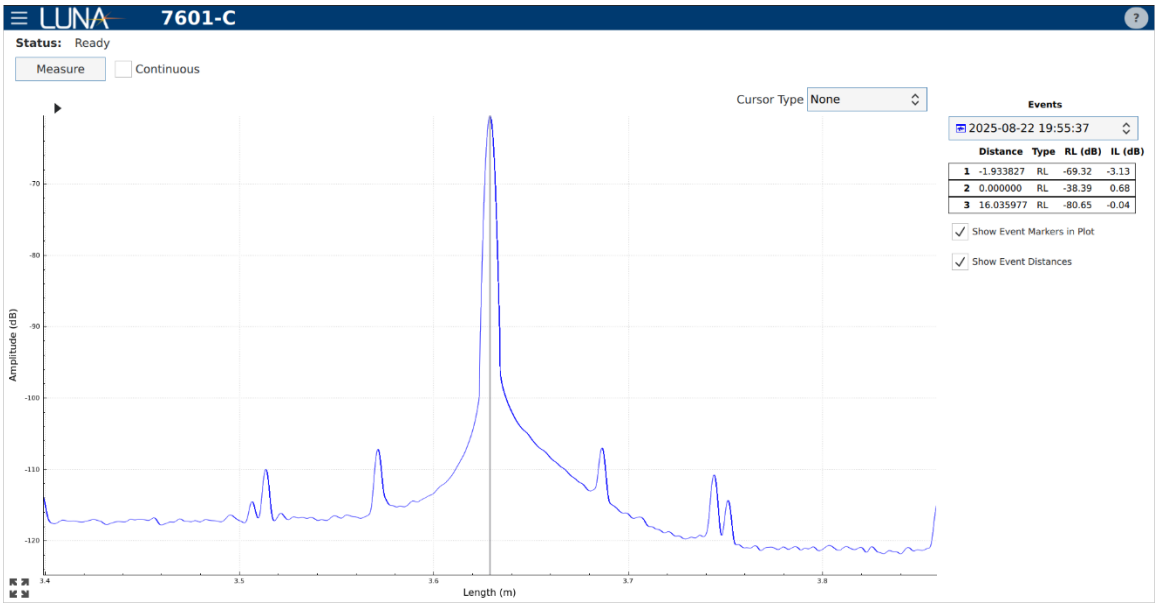
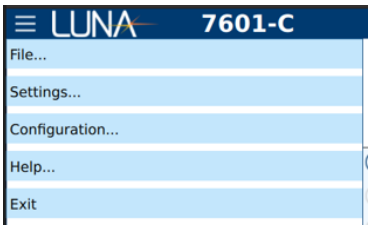


Figure 4-21 Double-clicking an event

4.5 Menu

4.5.1 Overview

Open the menu by clicking the three bars on the left top side of the user interface as shown in Figure 4-22. This will open the menu to perform file operations, settings, configuration management, help, and exiting the application.



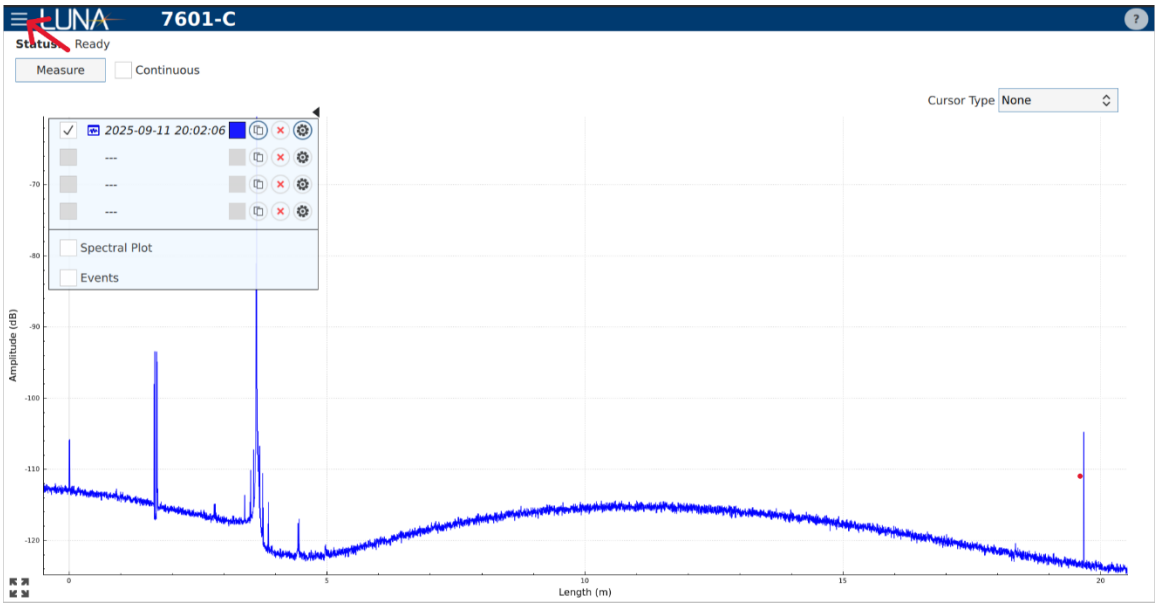


Figure 4-22 Menu

The following sections describe each menu item in detail.

4.5.2 File Operations

4.5.2.1 File Dialog

The file dialog as shown in Figure 4-23 is used to manage measurement files. Use the file dialog to navigate the file system, open measurement files, save measurement and TSV files, and delete measurement and TSV files.


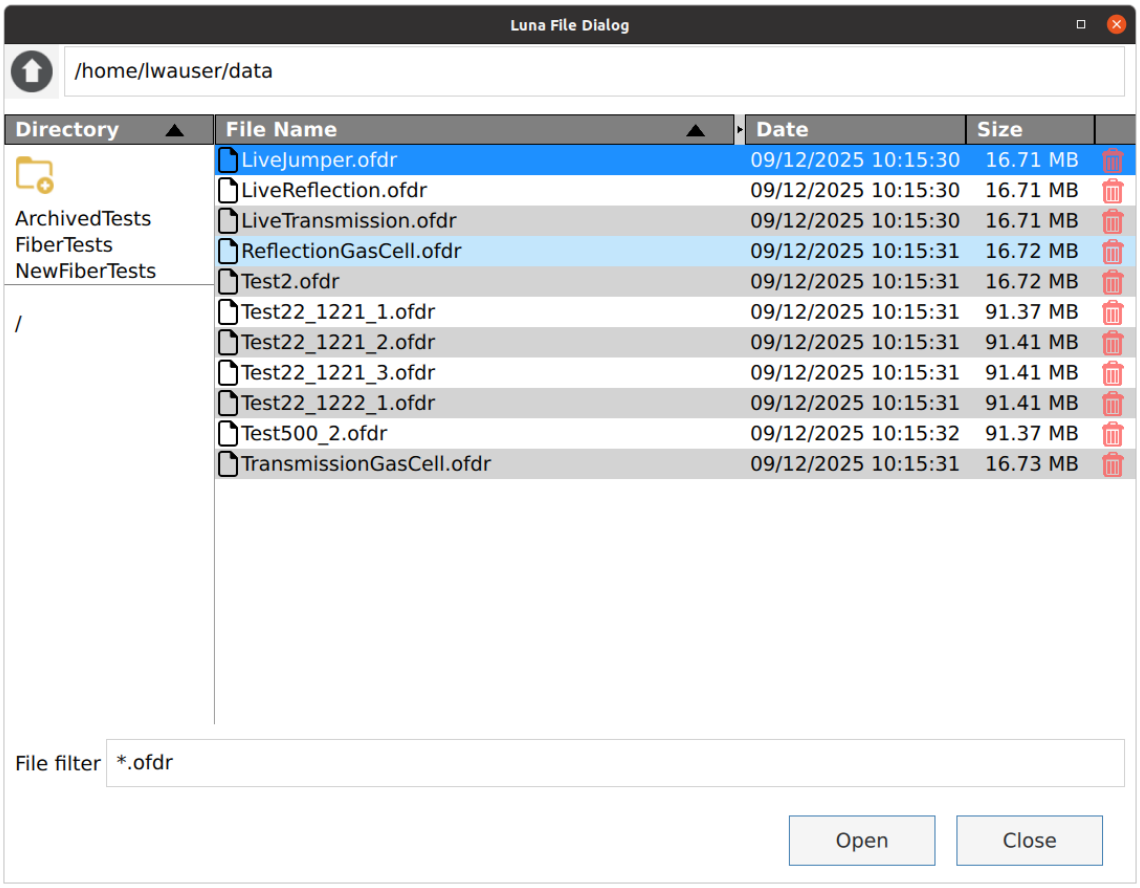



Figure 4-23 File Dialog

To navigate to a parent directory, click the up arrow next to the current directory name. To navigate to a child directory, click any of the directory names under the Directory list.



Under the directory names, it is possible to navigate to a different drive on the system. To create a new directory, click on the create directory icon . Each column may be sorted by clicking on the column header. To delete a file, click on the red trash can to the right of the file list. The File filter shows what is being filtered in the file list. This field is disabled and shows the file types that can be opened and saved.

4.5.2.2 Open



To open a measurement file, select File->Open to display the File Dialog as shown in Figure 4-23. Select the file which will be highlighted in blue and click the Open button to open the file. Both LWA measurement files (.ofdr) and OBR 4600 measurement files (.obr) can be opened. The file will be loaded in the first available trace as shown in Figure 4-24. In this example, "LiveJumper" was loaded into the second trace (the first available one) and the plot was updated to display the "LiveJumper" measurement. See section "4.1.3 Trace Settings" on how to manage traces that are loaded.

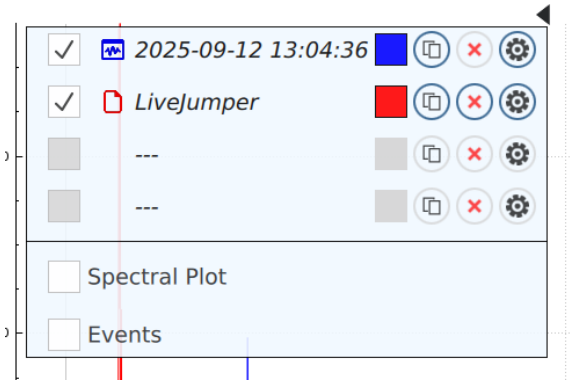


Figure 4-24 Loaded Trace File

4.5.2.3 Save



To save a measurement file and/or a TSV data file, select File->Save to display the File Dialog as shown in Figure 4-25. Type in a new file name or select an existing file name to overwrite. The extension ".ofdr" is added to the file name for a Measurement file, and ".tsv" for a TSV data file. The TSV file is a tab delimited spreadsheet file containing measurement data.

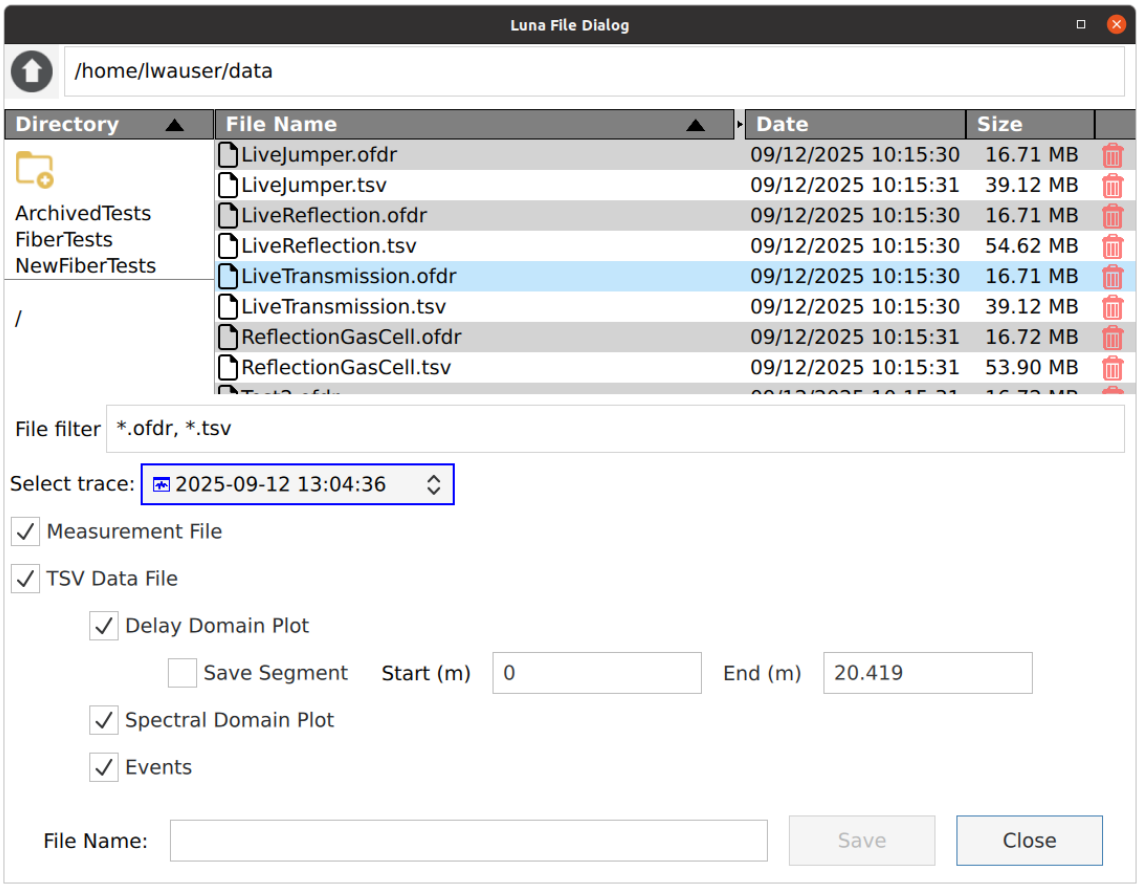



Figure 4-25 File Save Dialog

To save a measurement file, select the Measurement File checkbox 

. To save a TSV file, select the TSV Data File checkbox 

. For the TSV Data File, there are several options: Delay Domain Plot result, Spectral Domain Plot result and Events result. There is also an ability to specify a subsection of the Delay Domain Data to be saved in the TSV Data File by checking the Save Segment checkbox and entering the Start and End values. These options are shown in Figure 4-26.

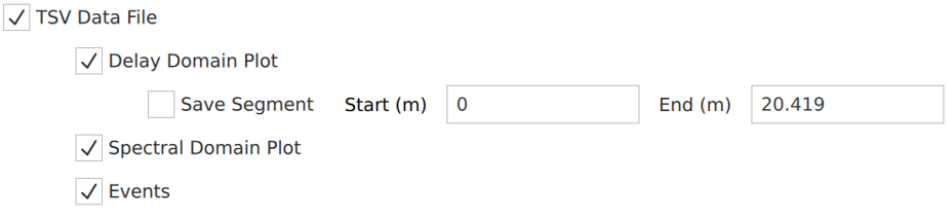


Figure 4-26 TSV Data File Options


If there is more than one trace, select the trace to be saved using the Select trace dropdown box as shown in Figure 4-27.



Figure 4-27 Selecting Trace to be Saved

4.5.3 Settings

4.5.3.1 Acquisition Settings

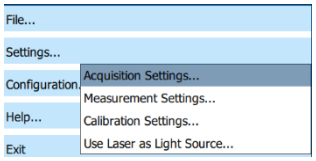

Select Settings->Acquisition Settings to change the acquisition settings on the instrument. Selecting Acquisition Settings displays the Acquisition Settings Dialog as shown in Figure 4-28.

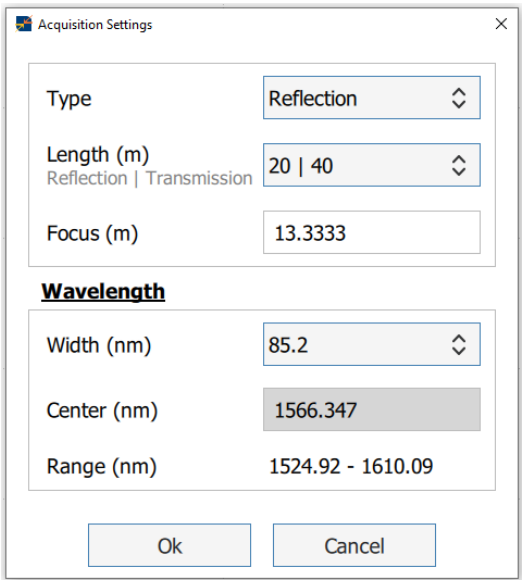


Figure 4-28 Acquisition Settings Dialog


Select the Acquisition Type by selecting either Reflection or Transmission from the Type Combo Box.

Select the acquisition length from the Length Combo Box. Each entry shows the length in reflection and then in transmission, as labeled under Length; for example, 20 | 40 is 20 m in reflection and 40 m in transmission. The lengths in meters (reflection) are: 20, 50, 100, 200, 500, 1000 and 2000. The 20 m range, and the 50 m range on LWA 7601-CL and 7601-O systems, are always available; the other ranges are available when their optional feature has been licensed. The length values are based on the display units selected.

The Focus field specifies a reference point near a peak that is used to optimize the data around that peak. Specify the focus point by typing the value in the field. The value is in the current display units.

On LWA 7601-CL and 7601-O systems, the Wavelength section selects the range of wavelengths that is acquired. Select a narrower width from the Width Combo Box to measure faster. Type a value in the Center field to move the range within the laser's sweep; the center cannot be changed at the full width. The Range field shows the resulting start and end wavelengths. The width returns to full when the length is changed. While a different length is selected but not yet applied, the Width and Center fields are unavailable.

4.5.3.2 Measurement Settings

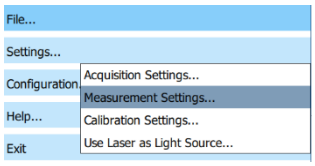

Select Settings->Measurement Settings to change settings while viewing and interacting with the displayed plots. Selecting Measurement Settings displays the Measurement Settings Dialog as shown in Figure 4-29.

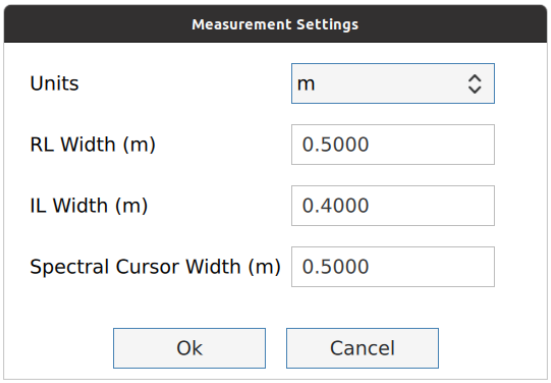



Figure 4-29 Measurement Settings Dialog

Selecting the Units changes the current display units including the delay plot x-axis. The default is meters (m). The available units are meters (m), millimeters (mm), inches (in), feet (ft) and nanoseconds (ns).

The RL Width and IL Width change the width of the integration regions that are used for return loss and insertion loss measurements. See section "4.2.2 Single Cursor."

The Spectral Cursor width specifies the data selection range of the spectral cursor if the Spectral Plot is enabled. See section "4.3.2 Spectral Cursor".

4.5.3.3 Calibration Settings

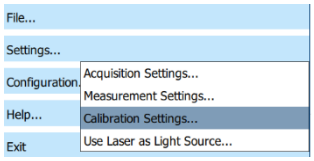

The instrument does not need to be calibrated each time it is started. The instrument should be recalibrated as needed. To recalibrate the instrument, select Settings->Calibration Settings. Selecting Calibration Settings displays the Calibration Settings Dialog as shown in Figure 4-30.

The Calibration Settings dialog displays the date of the current calibration and the date of the factory calibration. A single calibration covers every acquisition range.

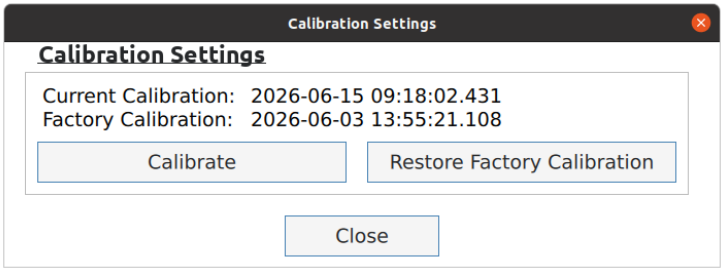




Figure 4-30 Calibration Settings Dialog

A new system delivered from Luna will be factory calibrated. To calibrate, click on the Calibrate button 

. To restore the factory calibration, click on the Restore Factory Calibration button 

. When calibrating, it is best to wait for approximately 15 minutes after turning on the instrument so that the instrument has time to warm up.

Calibration is available only in the 20 m and 50 m acquisition ranges. In the other ranges, the Calibrate and Restore Factory Calibration buttons are disabled and the dialog shows “Requires 20 m or 50 m mode”.


When you click Calibrate, the software guides you through the calibration:

1. Disconnect everything from the front panel when prompted, then click Ok.
2. When prompted, connect the Luna-supplied transmission calibration jumper, then click Ok.
3. Wait for the calibration to finish. The status shows Ready when it is complete.

NOTE: Recalibrate the instrument in the following cases:

- Once a new instrument is received.
- Any time the instrument is moved.
- When the ambient temperature changes approximately ±2°C (3.6°F).

4.5.3.4 Use Laser as Light Source

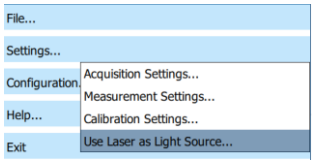

On LWA 7601-CL and 7601-O systems, the laser can be turned on at a single wavelength and used as a light source. Select Settings->Use Laser as Light Source to display the Use Laser as Light Source dialog as shown in Figure 4-31.

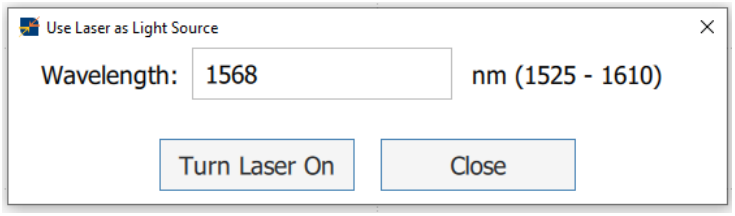



Figure 4-31 Use Laser as Light Source Dialog

Type the wavelength in the Wavelength field. The allowed range is shown to the right of the field. Click the Turn Laser On button 

to turn the laser on at that wavelength. While the laser is on, the dialog shows the wavelength, and measurements and settings are not available. To change the wavelength, type a new value and click Turn Laser On again. Click the Close button 


to turn the laser off and return to normal operation.

4.5.4 Configuration

System configuration can be saved, updated, or deleted through the configuration menus. A default configuration can be set to be used on system startup. The following settings are saved in a configuration:

- Display Units
- Group Index
- RL and IL Width
- Min and Max Event Locations
- RL and IL Threshold
- Apply Gaussian filter and Gaussian filter width
- Spectral Cursor Width
- Apply spectral Gaussian filter and spectral filter width

4.5.4.1 Load Configuration

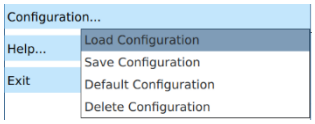

Selecting Configuration->Load Configuration displays the Load Configuration Dialog as shown in Figure 4-32.



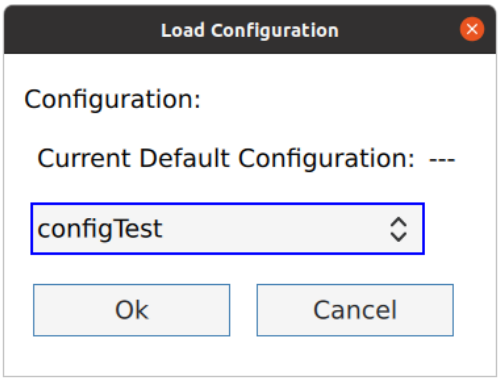


Figure 4-32 Load Configuration Dialog

Load a previously saved configuration by selecting the configuration from the combo box 

and clicking “Ok”.

4.5.4.2 Save Configuration

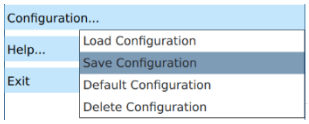

Selecting Configuration->Save Configuration displays the Save Configuration Dialog as shown in Figure 4-33.


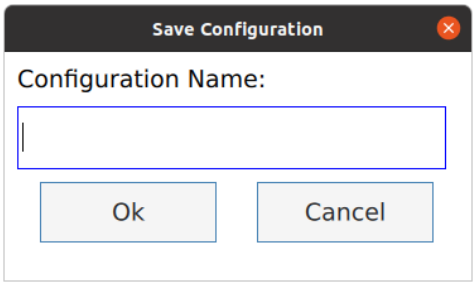


Figure 4-33 Save Configuration Dialog

Saving a configuration saves the settings listed above with the name specified in the Save Configuration Dialog. If the name already exists, a prompt will appear asking if it is okay to overwrite the previously saved configuration.

4.5.4.3 Default Configuration

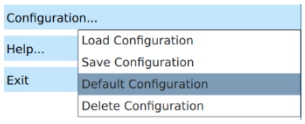

Selecting Configuration->Default Configuration displays the Default Configuration Dialog as shown in Figure 4-34.

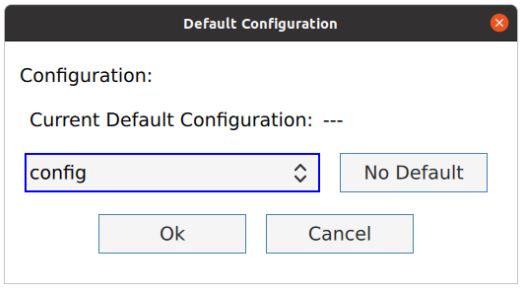




Figure 4-34 Default Configuration Dialog

The Default Configuration sets the configuration that the system will use on startup. If there is a default configuration already set, the name will be displayed in the "Current Default Configuration". Select the default configuration from the combo box 

. To clear the default configuration, select the No Default button 

.

4.5.4.4 Delete Configuration

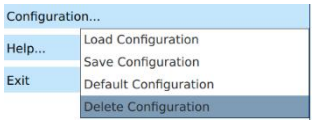

Selecting Configuration->Delete Configuration displays the Delete Configuration Dialog as shown in Figure 4-35.

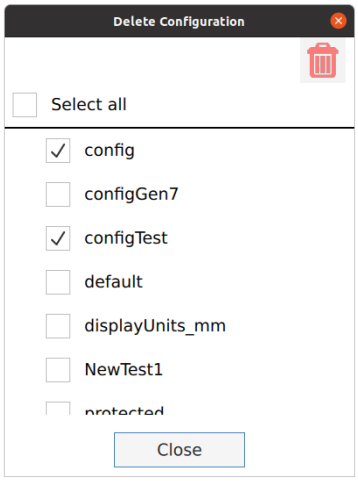


Figure 4-35 Delete Configuration Dialog

To delete one or more saved configurations, select the configurations to be deleted or check Select All Select all to select all the configurations. Click the red trash can to delete the selected configurations. A prompt will appear to confirm the deletion.

4.5.5 Help

4.5.5.1 Documentation

Select Help->Documentation to view system documentation and help as shown in Figure 4-36. These help documents can be accessed directly from the LWA 7600 software:

- **What's New**: Displays a list of the changes made for each version of the software.
- **User Guide**: Matching version of the LWA 7600 User's Guide (this document).
- **Setup Guide**: Instructions for how to set up the LWA 7600.


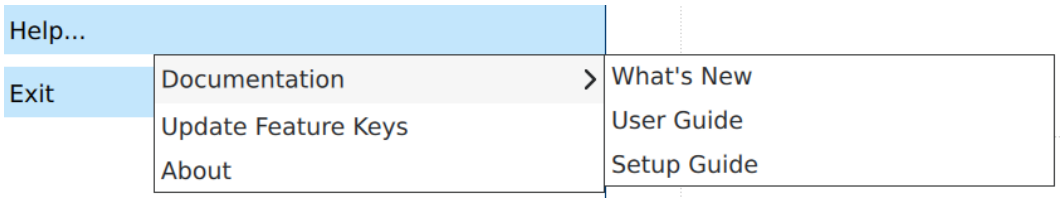



Figure 4-36 Help Documentation

4.5.5.2 Update Feature Keys

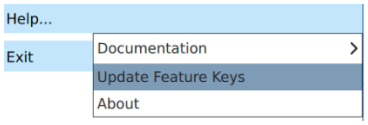

Select Help->Update Feature Keys to update the software with optionally purchased features. Once the file dialog is displayed, select the Luna provided feature key update file. The LWA software must be restarted after updating the feature keys on the instrument.

4.5.5.3 About

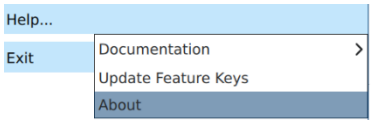

Select Help->About to display the About Dialog. This displays Luna contact information, the LWA 7600 software version information, connected hardware information, and a list of installed optional features as shown in Figure 4-37, Figure 4-38 and Figure 4-39.



Figure 4-37 About Dialog

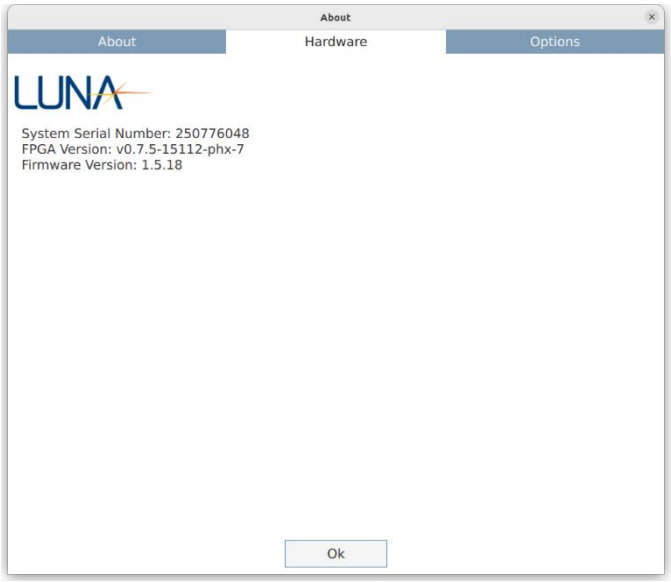


Figure 4-38 About Hardware Dialog

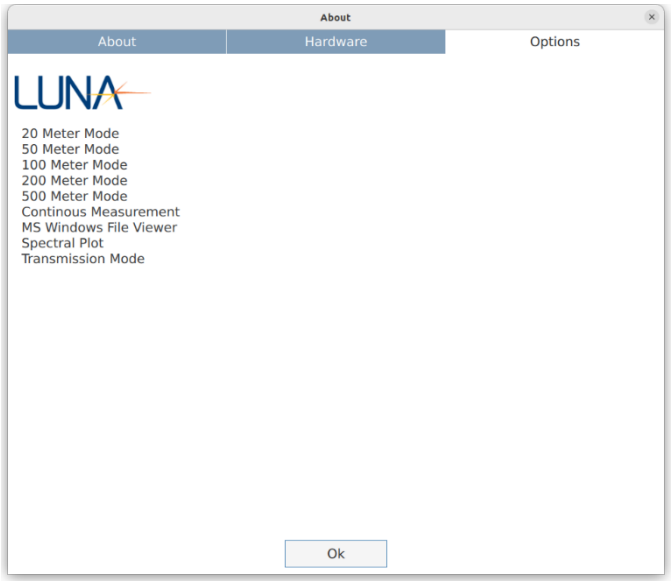


Figure 4-39 About Options Dialog

4.6 Remote User Interface

4.6.1 Installation

To install the remote user interface on Ubuntu Linux, run the file LWA_UI_v<version number>.run. Upon completion, a shortcut will be placed on the desktop to launch the LWA Remote User Interface.

To install the remote user interface on MS Windows, run the file LWAInstall.msi. Upon completion, a shortcut will be placed on the desktop and in the MS Windows Menu to launch the LWA Remote User Interface.

4.6.2 Disconnected Mode

The user software is able to be launched in disconnected mode. This can occur in two scenarios, either launching the user software on a system that does not have the controller software installed which is further described in Section 4.6.3 Remote Connection or launching the software without the instrument being connected as shown in Figure 4-40.

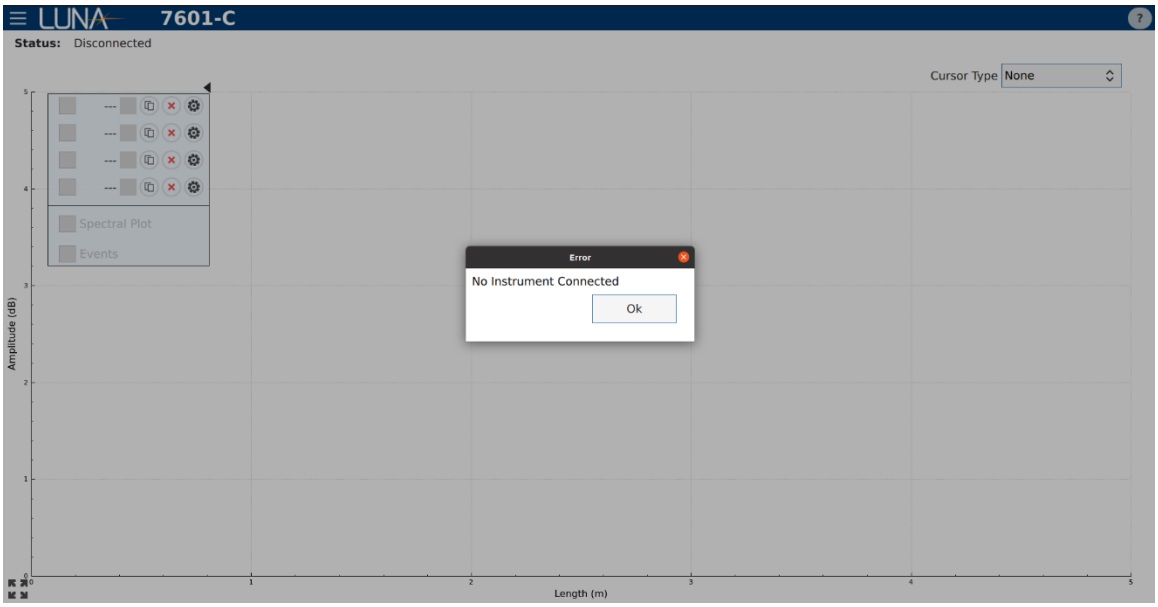


Figure 4-40 No Instrument Connected

In disconnected mode, the user interface operates solely in file viewing mode therefore the File Open and File Save options are available. See Section 4.5.2 File Operations. Since there is no instrument, Measurement Settings is the only settings option available as described in Section 4.5.3.2 Measurement Settings. Also, Help does not contain the ability to update feature keys and the Hardware and Options in the About screen are disabled.

NOTE: When running on a MS Windows system, an MS Windows File Viewer feature license is required to view measurement files while disconnected.

4.6.3 Remote Connection

The system allows remote connections in addition to the SCPI interface. The LWA 7600 supports the architecture as shown in Figure 4-41.

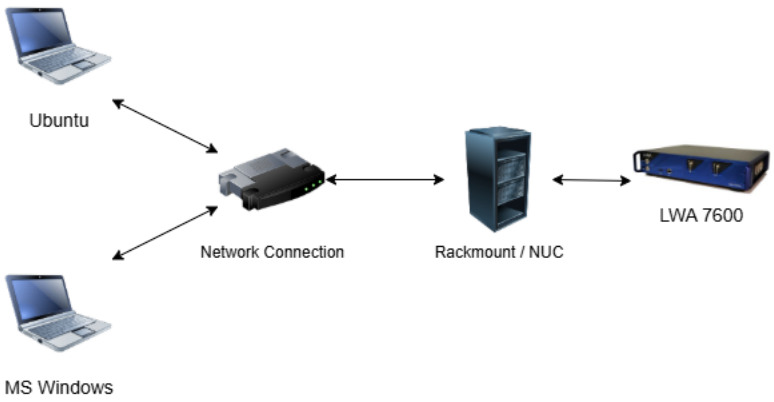


Figure 4-41 Remote Connection

The LWA 7600 Software can be installed on a Rackmount/NUC device supplied by Luna. The Rackmount/NUC is connected to the LWA 7600 as described in the Setup Guide. To use the LWA 7600 User Interface on the Rackmount/NUC itself, connect a mouse, keyboard and monitor to it.

The LWA 7600 User Interface can be installed on either a Ubuntu or MS Windows system. To connect to the LWA 7600 Software running on the Rackmount/NUC, start the LWA 7600 User Interface which will launch the user interface in a disconnected mode as shown in Figure 4-42. The connection button will show as a red disconnected icon when the user interface is not connected to an LWA system, referred to as the LWA Controller.

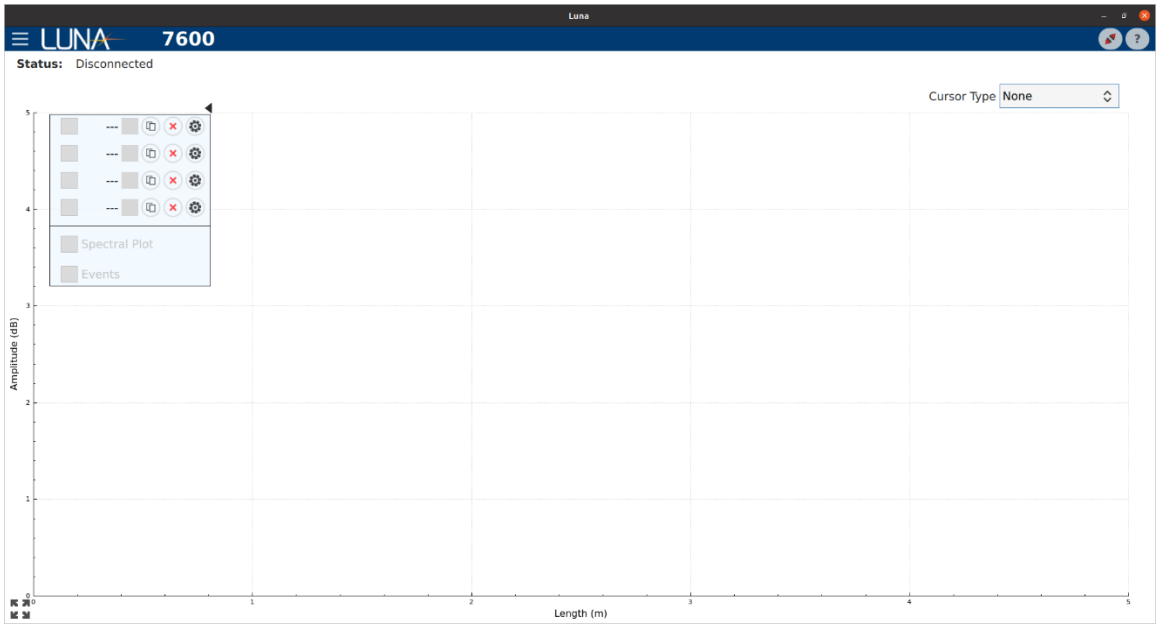


Figure 4-42 LWA User Interface Disconnected

To connect to a running LWA Controller, click on the connection button in the top right-hand corner of the user interface. This will display the Connection Manager Dialog as shown in Figure 4-43.

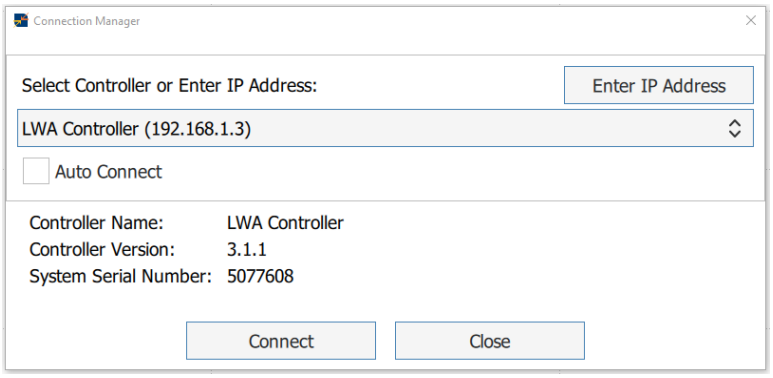



Figure 4-43 Connection Manager Dialog

Select the controller you wish to connect to from the Select Controller or Enter IP Address combo box. If the controller is not shown in the combo box, click the Enter IP Address button 

to type in a known controller IP Address. To always connect to the LWA Controller selected, check the Auto Connect checkbox 

. The UI in Auto Connect will automatically connect to the selected LWA Controller on startup. To stop using Auto Connect, uncheck the box. Click on the Connect button 

to connect.

Once connected, the connection icon  will turn green and show as connected. Clicking the Connection Button while connected displays the Connection Manager Dialog as shown in Figure 4-44.

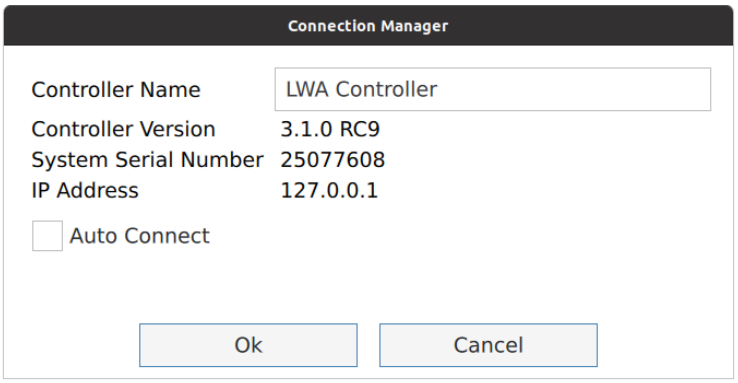


Figure 4-44 Connection Manager Dialog, Connected

The Connection Manager Dialog, while connected, provides a way to rename the LWA Controller and provides a way to set/unset Auto Connect. To rename the controller, edit the Controller Name field

.

While connected the LWA User Interface operates as described in this document.

5 SCPI Interface

5.1 Introduction to SCPI


SCPI commands may be sent to the controller over a network interface using the TCP/IP protocol. The IP address of the controller is displayed in the “About” settings page for your reference.

Port 5025 is used to communicate with the controller over a raw TCP/IP socket connection.

When using a Telnet client, you may press Alt+I to get a Telnet prompt (“>”).

Every response from the instrument, including error replies and binary data, ends with a null character (‘\0’).

5.2 Luna LWA 7600 SCPI Instrument Model

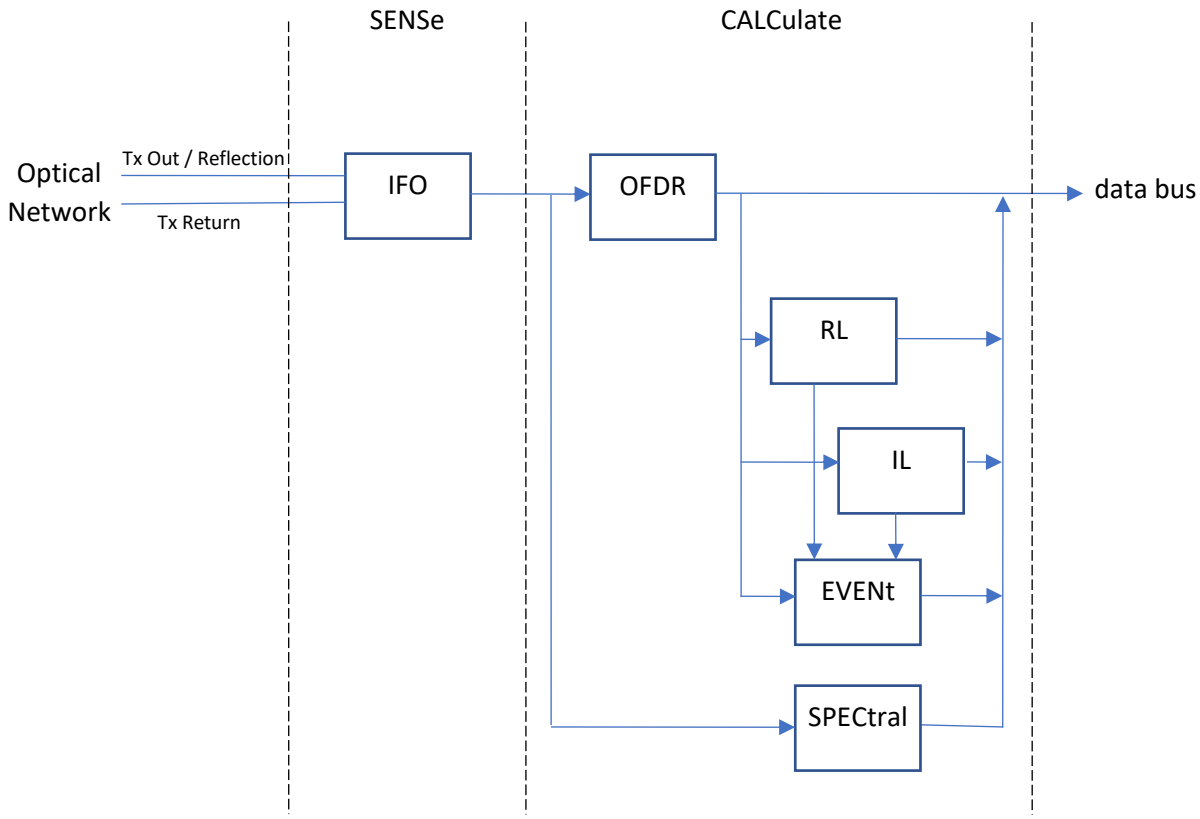

5.3 SCPI is Not a Data Streaming Protocol

SCPI should not be used while making continuous measurements. The SCPI protocol does not allow for the SCPI server to send unsolicited messages to the client. This means that the LWA 7600 software cannot send continuous measurement data as measurements are taken.

Instead, the client must send individual FETCh queries (for example, FETC:OFDR?, FETC:DIST?) which the server can respond to. However, there is no SCPI mechanism for knowing when a new measurement is available or for preventing the LWA 7600 from making a new measurement at the same time that the query is retrieving data.

To make and retrieve measurements as quickly as possible using SCPI, the client should send the INIT command to initiate a measurement, followed by the desired FETCh queries to retrieve data. The queries will not execute until the measurement has finished. This sequence can be repeated in a loop to acquire and retrieve multiple measurements.

5.4 Example SCPI Command Sequences

This section provides a few example command sequences to help demonstrate the use of SCPI with the Luna LWA 7600.

Keep in mind that it might be a good idea to follow each SCPI command or query with :SYST:ERR? to determine if an error was generated during the previous program message unit. For the sake of brevity, these examples don't demonstrate the use of the :SYST:ERR? query.

Refer to Section 5.5 for a complete list of supported SCPI commands.

5.4.1 Example 1: Take Sequential Measurements

DEL REFL # Use REFLection mode, not TRANsmission mode
LENG 20 # Use the 20 meter length (LENG 50 if 20 m is not available)
GIND 1.4682 # Set the group index to 1.4682
MEAS:RL? 3,0.05 # Take a measurement and get the return loss at a distance of 3m with a width of 0.05m
MEAS:RL? 3ft # Take a measurement and get the return loss at 3ft (still with a width of 0.05m)
MEAS:OFDR? # Take a measurement and return the amplitudes from the OFDR plot
MMEM:STOR ofdr,test1 # Store the measurement data to the file "test1.ofdr"
MMEM:STOR tsv_ose,test1 # Store all the measurement data to the file "test1.tsv"

5.4.2 Example 2: Get Multiple Results from a Single Measurement

```
DEL REFL              # Use REFLection mode, not TRANsmission mode
LENG 20               # Use the 20 meter length (LENG 50 if 20 m is not available)
GIND 1.4682           # Set the group index to 1.4682
CONF:RL DEF,0.05      # Set the return loss width to 0.05 meters
CONF:IL DEF,0.2       # Set the insertion loss width to 0.2 meters
CONF:SPEC DEF,0.5     # Set the spectral cursor width to 0.5 meters
INIT                  # Start a measurement
FETC:OFDR?            # Wait for the measurement to complete and get amplitudes in dB from the OFDR plot
FETC:DIST?            # Get distances in meters from the OFDR plot
FETC:SPEC? 1          # Get the return loss values in dB from the spectral plot with the spectral cursor at 1m
FETC:WAV?             # Get the wavelengths in nm from the spectral plot
FETC:EVEN?            # Get the event table
FETC:RL? 1.2          # Get the return loss at a distance of 1.2 meters from the unit
FETC:RL? 3ft          # Get the return loss at a distance of 3 feet from the unit
FETC:IL? 3.4m         # Get the insertion loss at a distance of 3.4 meters from the unit
```

5.4.3 Example 3: Get a Subset of the Measurement Data

```
DEL REFL              # Use REFLection mode, not TRANsmission mode
LENG 20               # Use the 20 meter length (LENG 50 if 20 m is not available)
INIT                  # Start a measurement
CONF:OFDR 0, 1.5, 2.5     # Configure FETC:OFDR? and DIST? queries to return data from 1.5m to 2.5m
FETC:OFDR?            # Wait for the measurement to complete and get amplitudes in dB from the OFDR plot
FETC:DIST?            # Get distances in meters from the OFDR plot
```

5.5 SCPI Command Reference

5.5.1 SENSe Subsystem

5.5.1.1 [:SENSe][:IFO]:DELay

```
> [:SENSe][:IFO]:DELay <CHARACTER PROGRAM DATA>
```

This command sets the measurement type. The parameter should be either TRANsmission or REFLection.

Note that IFO is an abbreviation for “interferometer”.

If a startup configuration file is enabled, then the *RST command sets the delay to the value from the startup configuration file. Otherwise, the *RST command sets the delay to REFLection.

5.5.1.2 [:SENSe][:IFO]:DELay?

```
> [:SENSe][:IFO]:DELay?
< <CHARACTER RESPONSE DATA>
```

This query returns the current measurement type. The response shall be either TRAN or REFL.

Note that IFO is an abbreviation for “interferometer”.

5.5.1.3 [:SENSe][:IFO]:LENGth

```
> [:SENSe][:IFO]:LENGth <numeric_value>[<SUFFIX>]
```

This command sets the measurement length. The parameter shall be 20m, 50m, 100m, 200m, 500m, 1000m or 2000m. The default units are meters (“m”). Although other units may be specified, the suffix (if provided) should be meters to guarantee that this setting is interpreted properly. Changing the length also sets the focus to two thirds of the new length.

Note that IFO is an abbreviation for “interferometer”.

The *RST command sets the measurement length to the startup length: 20m, or 50m on systems where 20m is not available.

The 20m length, and the 50m length on LWA 7601-CL and 7601-O systems, are always available. The other lengths are only available on units with the corresponding feature keys installed. A length that is not available returns error -224 “Illegal parameter value”.

If a previous length change is still in progress, the new length is applied after it finishes. While the instrument is starting up, this command returns error -221 “Settings conflict”.

In transmission, there is a difference between what the user interface displays and what is specified in the LENGth command. For example, the length of 20m will be displayed as an Acquisition Range of 40m.

5.5.1.4 [:SENSe][:IFO]:LENGth?

```
> [:SENSe][:IFO]:LENGth?
< <NR1>
```

This query returns the current measurement length. The response shall be 20, 50, 100, 200, 500, 1000 or 2000. The response is always in units of meters.

Note that IFO is an abbreviation for “interferometer”.

In transmission, there is a difference between what the user interface displays and what is returned by the LENGth? query. For example, the length of 20m will be displayed as an Acquisition Range of 40m.

5.5.1.5 [:SENSe][:IFO]:GINDex

```
> [:SENSe][:IFO]:GINDex <numeric_value>
```

This command sets the group index. The value must be from 1 to 4; otherwise error -222 “Data out of range” is returned.

Note that IFO is an abbreviation for “interferometer”.

If a startup configuration file is enabled, then the *RST command sets the group index to the value from the startup configuration file. Otherwise, the *RST command sets the group index to 1.4682.

5.5.1.6 [:SENSe][:IFO]:GINDex?

```
> [:SENSe][:IFO]:GINDex?
< <NR2>
```

This query returns the current group index.

Note that IFO is an abbreviation for “interferometer”.

5.5.1.7 [:SENSe][:IFO]:FOCUs

```
> [:SENSe][:IFO]:FOCUs <numeric_value>[<SUFFIX>]
```

This command sets the focus location. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”).

Note that IFO is an abbreviation for “interferometer”.

The *RST command sets the measurement length to the startup length (see [:SENSe][:IFO]:LENGth) and the focus to its default value.

5.5.1.8 [:SENSe][:IFO]:FOCUs?

```
> [:SENSe][:IFO]:FOCUs?
< <NR2>
```

This query returns the current focus location. The response is always in units of meters.

Note that IFO is an abbreviation for “interferometer”.

5.5.1.9 :SENSe:WAVelength:SPAN

```
> :SENSe:WAVelength:SPAN <numeric_value>[<SUFFIX>]|MINimum|MAXimum
```

This command sets the width of the acquisition window, in nanometers; an optional NM suffix is accepted. The widths allowed are the full width for the current measurement length, and that width halved up to five times. Any other value is set to the nearest allowed width. MAXimum selects the full width and MINimum the narrowest width. A narrower width measures faster.

When the width is narrowed, the current center is kept if possible; otherwise it is moved so the window stays within the full range. At the full width, the window uses the default center for the measurement length. The command completes once the change is done and a new measurement has been taken.

This command is only available on LWA 7601-CL and 7601-O systems. On other systems, and while the laser is on as a light source, it returns error -221 “Settings conflict”.

A change of measurement length returns the window to the full width. The *RST command also returns the window to the full width.

5.5.1.10 :SENSe:WAVelength:SPAN?

```
> :SENSe:WAVelength:SPAN? [MINimum|MAXimum]
< <NR2>
```

This query returns the width of the acquisition window in nanometers. With MINimum or MAXimum, it returns the narrowest or the full width for the current measurement length.

This query is only available on LWA 7601-CL and 7601-O systems.

5.5.1.11 :SENSe:WAVelength:CENTer

```
> :SENSe:WAVelength:CENTer <numeric_value>[<SUFFIX>]|MINimum|MAXimum
```

This command sets the center wavelength of the acquisition window, in nanometers; an optional NM suffix is accepted. A value outside the range that keeps the window within the full range is set to the nearest value in that range. MINimum and MAXimum select the lowest and highest center for the current width. The command completes once the change is done and a new measurement has been taken.

At the full width the center cannot be changed, and this command returns error -221 “Settings conflict”. It also returns error -221 on systems other than LWA 7601-CL and 7601-O, and while the laser is on as a light source.

5.5.1.12 :SENSe:WAVelength:CENTer?

```
> :SENSe:WAVelength:CENTer? [MINimum|MAXimum]
< <NR2>
```

This query returns the center wavelength of the acquisition window in nanometers. With MINimum or MAXimum, it returns the lowest or highest center that can be set at the current width.

This query is only available on LWA 7601-CL and 7601-O systems.

5.5.1.13 :SENSe:WAVelength:STARt?

```
> :SENSe:WAVelength:STARt?
< <NR2>
```

This query returns the shortest wavelength of the acquisition window in nanometers.

This query is only available on LWA 7601-CL and 7601-O systems.

5.5.1.14 :SENSe:WAVelength:STOP?

```
> :SENSe:WAVelength:STOP?
< <NR2>
```

This query returns the longest wavelength of the acquisition window in nanometers.

This query is only available on LWA 7601-CL and 7601-O systems.

5.5.2 SOURce Subsystem

5.5.2.1 :SOURce:WAVelength

```
> :SOURce:WAVelength <numeric_value>[<SUFFIX>]
```

This command sets the wavelength of the laser when it is used as a light source. The value is in nanometers; an optional NM suffix is accepted. The allowed range is 1525 to 1610 nm on LWA 7601-CL systems and 1270 to 1340 nm on LWA 7601-O systems. A value outside the range returns error -222 “Data out of range”.

When the output is off, the wavelength is stored and used by the next :OUTPut ON command. When the output is on, the laser moves to the new wavelength, and the command completes once it is there.

This command is only available on LWA 7601-CL and 7601-O systems. On other systems it returns error -221 “Settings conflict”.

The *RST command sets the wavelength to the middle of the allowed range.

5.5.2.2 :SOURce:WAVelength?

```
> :SOURce:WAVelength? [MINimum|MAXimum]
< <NR2>
```

This query returns the laser wavelength in nanometers. While the output is on, it returns the wavelength the laser is set to; otherwise it returns the stored wavelength. With MINimum or MAXimum, it returns the lowest or highest allowed wavelength.

This query is only available on LWA 7601-CL and 7601-O systems.

5.5.3 OUTPut Subsystem

5.5.3.1 :OUTPut[:STATe]

```
> :OUTPut[:STATe] <boolean>
```

This command turns the laser on or off as a light source. A <boolean> value of 1 or ON turns the laser on at the wavelength set by :SOURce:WAVelength. A value of 0 or OFF turns it off and returns the instrument to normal measurements. The command completes once the laser is on, or once normal measurements have resumed.

While the output is on, the following commands return error -221 “Settings conflict”: :INITiate, :FETCh, :READ, :MEASure, [:SENSe][:IFO]:LENGth, [:SENSe][:IFO]:DELay, [:SENSe][:IFO]:GINDex, [:SENSe][:IFO]:FOCUs, :OFDR:FILTer:GAUSsian, :SENSe:WAVelength:SPAN, :SENSe:WAVelength:CENTer, :MMEMory:STORe, :MMEMory:LOAD and *RCL. Queries (such as *IDN?, :SYSTem:ERRor? and [:SENSe][:IFO]:LENGth?) and the :CONFigure commands can still be used, except :OFDR:FILTer:GAUSsian:STATe? and :OFDR:FILTer:GAUSsian:WIDTh?, which also return error -221 while the output is on.

This command is only available on LWA 7601-CL and 7601-O systems. On other systems, :OUTPut ON returns error -221 “Settings conflict”.

The *RST command turns the output off.

5.5.3.2 :OUTPut[:STATe]?

```
> :OUTPut[:STATe]?
< <NR1>
```

This query returns 1 if the laser is on as a light source (whether it was turned on over SCPI or from the user interface), and 0 otherwise.

5.5.4 CALCulate Subsystem

5.5.4.1 :OFDR:FILTer:GAUSsian[:STATe]

```
> :OFDR:FILTer:GAUSsian[:STATe] <boolean>
```

This command turns the Gaussian filter on or off on the OFDR data plot. A <boolean> value of 1 or ON turns on the Gaussian filter while a value of 0 or OFF turns it off.

Note that OFDR is an alias for CALCulate. These program mnemonics may be used interchangeably.

If a startup configuration file is enabled, then the *RST command sets the Gaussian filter state to the value from the startup configuration file. Otherwise, the *RST command turns the Gaussian filter on.

5.5.4.2 :OFDR:FILTer:GAUSsian[:STATe]?

```
> :OFDR:FILTer:GAUSsian[:STATe]?
< <NR1>
```

This query returns the current state of the Gaussian filter. The response shall either be 0 to indicate the filter is turned off or 1 to indicate it is turned on.

Note that OFDR is an alias for CALCulate. These program mnemonics may be used interchangeably.

5.5.4.3 :OFDR:FILTer:GAUSsian:WIDTh

```
> :OFDR:FILTer:GAUSsian:WIDTh <numeric_value>
```

This command sets the filter width for the Gaussian filter to the specified value. The value is always in millimeters; any unit suffix is ignored. The width is set to the nearest available width: 0.16, 0.32, 0.64, 1.28, 2.56, 5.12 or 10.24 mm.

Note that OFDR is an alias for CALCulate. These program mnemonics may be used interchangeably.

If a startup configuration file is enabled, then the *RST command sets the Gaussian filter width to the value from the startup configuration file. Otherwise, the *RST command sets the Gaussian filter width to 10.24mm.

5.5.4.4 :OFDR:FILTer:GAUSsian:WIDTh?

```
> :OFDR:FILTer:GAUSsian:WIDTh?
< <NR2>
```

This query returns the current filter width of the Gaussian filter. The response is always in units of millimeters.

Note that OFDR is an alias for CALCulate. These program mnemonics may be used interchangeably.

5.5.5 Measurement Instructions

The :FETCh, :READ and :MEASure queries return error -230 “Data corrupt or stale” when there is no measurement to return: when no measurement has been taken yet (for example, on an instrument that needs to be calibrated), or when the requested measurement was not taken.

5.5.5.1 :CONFigure?

```
> :CONFigure?
< <function> <parameters>
```

This query returns the measurement function and configuration parameters for the most recently configured measurement function. The parameters follow the format of the corresponding CONFigure query for the indicated measurement function.

If no measurement function has been configured, or if the last one was configured by :MEASure:GD?, then this query produces no response other than the response message terminator.

5.5.5.2 :CONFigure:RL

```
> :CONFigure:RL <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
```

This command sets return loss as the current measurement and optionally sets the current return loss center location to the value of the first parameter and the return loss width to the value of the second parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

If a startup configuration file is enabled, then the *RST command sets the return loss center location and width to the values from the startup configuration file. Otherwise, the *RST command sets the return loss center location to 0.0m and the width to 0.05m.

5.5.5.3 :CONFigure:RL?

```
> :CONFigure:RL?
< <NR2>,<NR2>
```

This query returns the current return loss configuration. The first response is the current return loss center location and the second response is the current return loss width. Both values are always in units of meters.

5.5.5.4 :CONFigure:IL

```
> :CONFigure:IL
  <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
```

This command sets insertion loss as the current measurement and optionally sets the current insertion loss center location to the value of the first parameter, the insertion loss width to the value of the second parameter and the return loss width to the value of the third parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

If a startup configuration file is enabled, then the *RST command sets the insertion loss center location and width to the values from the startup configuration file. Otherwise, the *RST command sets the insertion loss center location to 0.0m and the width to 0.2m.

5.5.5.5 :CONFigure:IL?

```
> :CONFigure:IL?
< <NR2>,<NR2>,<NR2>
```

This query returns the current insertion loss configuration. The first response is the current insertion loss center location, the second response is the current insertion loss width and the third response is the current return loss width. All values are always in units of meters.

5.5.5.6 :CONFigure:OFDR

```
> :CONFigure:OFDR [<measurement id>],[<start>,<end>]
```

This command sets the amplitude data from the OFDR graph as the current measurement.

The optional <measurement id> parameter is an integer indicating which measurement should be returned from FETC:OFDR? and FETC:DIST? queries. Currently the only valid value is 0.

The optional <start> and <end> parameters are floating point values indicating the start and end location for the measurement segment that will be returned.

5.5.5.7 :CONFigure:OFDR?

```
> :CONFigure:OFDR?
  < <NR1>,<NR2>,<NR2>
```

This query returns the measurement id and the start and end locations, in meters, used by the :FETCh:OFDR? and :FETCh:DISTance? queries.

5.5.5.8 :CONFigure:DISTance

```
> :CONFigure:DISTance [<measurement id>],[<start>,<end>]
```

This command sets the distance data from the OFDR graph as the current measurement.

The optional <measurement id> parameter is an integer indicating which measurement should be returned from FETC:OFDR? and FETC:DIST? queries. Currently the only valid value is 0.

The optional <start> and <end> parameters are floating point values indicating the start and end location for the measurement segment that will be returned.

5.5.5.9 :CONFigure:DISTance?

```
> :CONFigure:DISTance?
  < <NR1>,<NR2>,<NR2>
```

This query returns the measurement id and the start and end locations, in meters, used by the :FETCh:OFDR? and :FETCh:DISTance? queries. It returns the same values as :CONFigure:OFDR?.

5.5.5.10 :CONFigure:SPECtral

```
> :CONFigure:SPECtral <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
```

This command sets the spectral data as the current measurement and optionally sets the current spectral center location to the value of the first parameter and the current spectral width to the value of the second parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

If a startup configuration file is enabled, then the *RST command sets the spectral center location and width to the values from the startup configuration file. Otherwise, the *RST command sets the spectral center location to 0.0m and the width to 0.5m.

This command is only available on units with the spectral feature key installed.

5.5.5.11 :CONFigure:SPECtral?

```
> :CONFigure:SPECtral?
< <NR2>,<NR2>
```

This query returns the current spectral configuration. The first response is the current spectral center location and the second response is the current spectral width. Both values are always in units of meters.

This query is only available on units with the spectral feature key installed.

5.5.5.12 :CONFigure:EVENt

```
> :CONFigure:EVENt <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>],
  <numeric_value>[dB],<numeric_value>[dB]
```

This command sets event detection as the current measurement and optionally sets the minimum event location to the first parameter, the maximum event location to the second parameter, the RL threshold to the third parameter and the IL threshold to the fourth parameter. The default units for the minimum and maximum event locations are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). The default units for the RL and IL thresholds are decibels (“dB”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault. The RL threshold must be from 1 to 20 dB and the IL threshold from -10 to -1 dB; otherwise error -222 “Data out of range” is returned.

If a startup configuration file is enabled, then the *RST command sets the minimum event location, maximum event location, RL threshold and IL threshold to the values from the startup configuration file. Otherwise, the *RST command sets the minimum event location to -1.0m, the maximum event location to 20.0m, the RL threshold to 4.0dB and the IL threshold to -2.0dB.

5.5.5.13 :CONFigure:EVENt?

```
> :CONFigure:EVENt?
< <NR2>,<NR2>,<NR2>,<NR2>
```

This query returns the current event configuration. The first response is the minimum event location, the second response is the maximum event location, the third response is the RL threshold

and the fourth response is the IL threshold. The minimum and maximum event locations are always in units of meters and the RL and IL thresholds are always in units of decibels.

5.5.5.14 :BINary

```
> :BINary <boolean>
```

This command turns the binary output mode on or off. A <boolean> value of 1 or ON turns on the binary output while a value of 0 or OFF turns it off.

This command affects the following FETCh commands:

- :FETCh:OFDR?
- :FETCh:DISTance?
- :FETCh:SPECtral?
- :FETCh:GD?
- :FETCh:WAVelength?

The default for the BINary command is off where the above commands will output data in ASCII format.

When binary is turned on, the above commands will output data in a length-prefixed array of IEEE-754 floating-point values. The first 4 bytes are an unsigned 32-bit integer count in little-endian byte order representing the number of data points. This is followed by the count of consecutive values in little-endian byte order, each 4 bytes (single-precision, 32-bit) or 8 bytes (double-precision, 64-bit) as set by :FORMat:DATA. There are no delimiters such as commas or terminators inside the binary output.

5.5.5.15 :BINary?

```
> :BINary?
< <CHARACTER RESPONSE DATA>
```

This query returns the current state of the binary output. The response shall either be off to indicate binary output is turned off or on to indicate it is turned on.

5.5.5.16 :FORMat:DATA

```
> :FORMat:DATA REAL,32|REAL,64
```

This command sets the size of the values in the binary output (see :BINary). REAL,32 outputs IEEE-754 single-precision (32-bit) values and REAL,64 outputs IEEE-754 double-precision (64-bit) values. The default is REAL,32.

Use REAL,64 with :FETCh:DISTance? at measurement lengths above 1000 m. At these lengths, 32-bit values do not have enough precision to give every point a different distance.

This command does not turn the binary output on or off; use :BINary for that. The *RST command does not change this setting.

5.5.5.17 :FORMat:DATA?

```
> :FORMat:DATA?
< <CHARACTER RESPONSE DATA>
```

This query returns the size of the values in the binary output: REAL,32 or REAL,64.

5.5.5.18 :FETCh?

```
> :FETCh?
< (see the corresponding :FETCh:<function>? query for the response format)
```

The last measurement function FETChed, READ or MEASured will be fetched.

If no measurement function has been used, then this query produces no response other than the response message terminator.

5.5.5.19 :FETCh:RL?

```
> :FETCh:RL? <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
< <NR2>
```

This query waits for a measurement to complete and returns the measured return loss in dB. The command also optionally sets the return loss center location to the value of the first parameter and the return loss width to the value of the second parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

5.5.5.20 :FETCh:IL?

```
> :FETCh:IL?
<numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
< <NR2>
```

This query waits for a measurement to complete and returns the measured insertion loss in dB. The command also optionally sets the insertion loss center location to the value of the first parameter and the insertion loss width to the value of the second parameter and the return loss width to the value of the third parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

5.5.5.21 :FETCh:OFDR?

```
> :FETCh:OFDR? [<measurement id>],[<start>,<end>]
< <NR2>{,<NR2>}
```

This query waits for a measurement to complete and returns the amplitude data from the OFDR graph. Each data point is always in units of decibels. Note that the corresponding distance coordinate values for this data can be returned by using the :FETCh:DISTance? query.

The optional <measurement id> parameter is an integer indicating which measurement should be returned. Currently the only valid value is 0.

The optional <start> and <end> parameters are floating point values indicating the start and end location for the measurement segment that will be returned.

5.5.5.22 :FETCh:DISTance?

```
> :FETCh:DISTance? [<measurement id>],[<start>,<end>]
< <NR2>{,<NR2>}
```

This query waits for a measurement to complete and returns the distance data from the OFDR graph. Each data point is always in units of meters. Note that the corresponding amplitude coordinate values for this data can be returned by using the :FETCh:OFDR? query.

The optional <measurement id> parameter is an integer indicating which measurement should be returned. Currently the only valid value is 0.

The optional <start> and <end> parameters are floating point values indicating the start and end location for the measurement segment that will be returned.

5.5.5.23 :FETCh:SPECtral?

```
> :FETCh:SPECtral? <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
< <NR2>{,<NR2>}
```

This query waits for a measurement to complete and returns the return loss data from the spectral graph. Each data point is always in units of decibels. Note that the corresponding wavelength coordinate values for this data can be returned by using the :FETCh:WAVelength? query. The command also optionally sets the current spectral center location to the value of the first parameter, and the current spectral width to the value of the second parameter. The default units are meters (“m”). Other possible units include millimeters (“mm”), feet (“ft”), and inches (“in”). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

This query is only available on units with the spectral feature key installed.

5.5.5.24 :FETCh:GD?

```
> :FETCh:GD? <numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>]
< <NR2>{,<NR2>}
```

This query waits for a measurement to complete and returns the group delay data from the spectral graph. Each data point is always in units of nanoseconds. In reflection, the group delay is the round-trip delay; in transmission, it is the one-way delay. See Group Delay in Theory of Operation. Note that the corresponding wavelength coordinate values for this data can be returned by using the :FETCh:WAVelength? query. The command also optionally sets the current spectral center location to the value of the first parameter, and the current spectral width to the value of the second parameter. The default units are meters ("m"). Other possible units include millimeters ("mm"),

feet ("ft"), and inches ("in"). Parameters can also be defaulted to their current value by omitting them from right-to-left, or by using the special parameter DEFault.

This query is only available on units with the spectral feature key installed.

5.5.5.25 :FETCh:WAVelength?

```
> :FETCh:WAVelength?
< <NR2>{,<NR2>}
```

This query waits for a measurement to complete and returns the wavelength data from the spectral graph. Each data point is always in units of nanometers. Note that the corresponding return loss coordinate values for this data can be returned by using the :FETCh:SPECtral? query.

This query is only available on units with the spectral feature key installed.

5.5.5.26 :FETCh:EVENt?

```
> :FETCh:EVENt?
[<numeric_value>[<SUFFIX>],<numeric_value>[<SUFFIX>],<numeric_value>[dB],<numer
ic_value>[dB]]
< <EXPR>{,<EXPR>}
```

This query waits for a measurement to complete and returns a list of events for the current measurement. The query also optionally sets the minimum event location, maximum event location, RL threshold and IL threshold, as described for :CONFigure:EVENt. Each <EXPR> result is formatted as:

(<NR2>,<NR1>,<NR2>,<NR2>)

The values in each <EXPR> represent, in order, the following values:

- location of the event in meters
- for reflection, event type as an integer (0 for a return loss event, 1 for an insertion loss event)
- for transmission, event type as an integer (0 for an insertion loss event)
- for reflection, return loss at the event location in dB
- insertion loss at the event location in dB (in transmission, each <EXPR> has only three values, and this is the third)

5.5.5.27 :READ[:<function>]?

```
> :READ[:<function>]? <parameters>
< (see the corresponding :FETCh:<function>? query for the response format)
```

This query starts a measurement (as :INITiate does) and then returns the result (as :FETCh[:<function>]? does).

If the <function> is not specified in the query, then the last measurement function FETCHed, READ or MEASured will be read.

If no measurement function has been used, then this query produces no response other than the response message terminator.

5.5.5.28 :MEASure[:<function>]?

```
> :MEASure[:<function>]? <parameters>
< (see the corresponding :FETCh:<function>? query for the response format)
```

This query configures the measurement function with the given parameters (as :CONFigure does), then starts a measurement and returns the result (as :READ does).

If the <function> is not specified in the query, then the most recently configured measurement function (see :CONFigure?) will be measured. The supported functions are RL, IL, OFDR, SPECtral, GD and EVENt.

If no measurement function has been used, then this query produces no response other than the response message terminator.

5.5.6 TRIGger Subsystem

5.5.6.1 :INITiate[:ALL]

```
> :INITiate[:ALL]
```

This command acquires a single measurement. Error -213 “Init ignored” is generated if the instrument is not ready or if a measurement is already in progress.

If no measurement has been taken yet, for example on an instrument that needs to be calibrated, this command returns error -230 “Data corrupt or stale”.

5.5.7 MMEMory Subsystem

5.5.7.1 :MMEMory:LOAD:STATe

```
> :MMEMory:LOAD:STATe <numeric_value>,<file_name>
```

This command loads instrument configuration data from a file. The <numeric_value> is the memory register number where the configuration data will be loaded into the instrument. Memory register 0 represents the current configuration in use by the instrument. Memory register 1 represents the default settings that will be used whenever the LWA software is started. The <file_name> is the name of the configuration file to load, without quotes. If the filename does not end with the extension “.config”, then “.config” will be appended to the filename.

5.5.7.2 :MMEMory:STORe:STATe

```
> :MMEMory:STORe:STATe <numeric_value>,<file_name>
```

This command saves instrument configuration data to a file. The <numeric_value> is the memory register number containing the instrument configuration to be saved to the file. Memory register 0 represents the current configuration in use by the instrument. With memory register 1, the command makes the existing <file_name> the startup configuration file (the configuration used whenever the LWA software is started); error -256 "File name not found" is returned if the file does not exist. The <file_name> is the name of the configuration file to save, without quotes. If the filename does not end with the extension ".config", then ".config" will be appended to the filename.

5.5.7.3 :MMEMory:STORe[:CUSTom]

```
> :MMEMory:STORe[:CUSTom] <label>,<file_name>,[<measurement
id>],[<start>,<end>]
```

This command stores the current measurement data to a file. The <label> identifies what type of file will be stored:

OFDR	OFDR measurement file
TSV	Tab-separated value file containing only the header
TSV_E	Tab-separated value file containing the events detected
TSV_S	Tab-separated value file containing the spectral data
TSV_SE	Tab-separated value file containing the spectral data and the events detected
TSV_O	Tab-separated value file containing the OFDR data
TSV_OE	Tab-separated value file containing the OFDR data and the events detected
TSV_OS	Tab-separated value file containing the OFDR data and the spectral data
TSV_OSE	Tab-separated value file containing all the data

The <file_name> is the name of the file to save, without quotes. If the <label> is OFDR and the filename does not end with the extension ".ofdr", then ".ofdr" will be appended to the filename. If <label> starts with TSV and the filename does not end with the extension ".tsv", then ".tsv" will be appended to the filename.

The optional <measurement id> parameter is an integer indicating which measurement should be saved. Currently the only valid value is 0.

The optional <start> and <end> parameters are floating point values indicating the start and end location for the measurement segment that should be saved. This only affects the OFDR data written to the TSV file.

The command completes once the file has been completely written, which can take several seconds for a large file.

The spectral data written to a TSV file, including the group delay, is calculated at the spectral cursor set by :CONFigure:SPECtral.

If no measurement has been taken yet, this command returns error -230 “Data corrupt or stale”.

5.5.8 SYSTem Subsystem

5.5.8.1 :SYSTem:ERRor[:NEXT]?

```
> :SYSTem:ERRor[:NEXT]?
< <NR1>,<STRING RESPONSE DATA>
```

This query removes the next item from the Error/Event Queue and returns it in the response.

The <NR1> number is an Error/Event number in the range of -32768 through 32767. The <STRING RESPONSE DATA> is a description of the Error/Event.

Each SCPI connection has its own Error/Event Queue, which holds up to 10 entries. Errors are returned oldest first. If an error occurs while the queue is full, the last entry is replaced with -350,“Queue overflow”.

Each error also sets a bit in the Standard Event Status Register (see *ESR?): bit 5 for a command error (-100 to -199), bit 4 for an execution error (-200 to -299), and bit 3 for a device-dependent error (-300 to -399).

If there are no entries in the Error/Event Queue, then the response is:

0,”No error”

The Error/Event Queue shall be cleared by the *CLS command or by reading the last item from the queue.

5.5.8.2 :SYSTem:VERSion?

```
> :SYSTem:VERSion?
< <NR2>
```

This query returns the SCPI version number with which the instrument complies.

The response is always 1999.0.

5.5.9 STATus Subsystem

5.5.9.1 :STATus:OPERation:CONDition?

```
> :STATus:OPERation:CONDition?
< <NR1>
```

This query returns the value of the OPERation:CONDition register. The response shall be in the range of 0 through 32767.

The SCPI standard defines the following bits for the OPERation:CONDition register.

Bit	Meaning
	1 if the instrument is…
0: CALibrating	…currently performing a calibration
1: SETTling	…waiting for signals it controls to stabilize enough to begin measurements
2: RANGing	…currently changing its range
3: SWEeping	…performing a sweep operation that's still in progress
4: MEASuring	…actively measuring
5: Waiting for TRIG	…in a "wait for trigger" state of the trigger model
6: Waiting for ARM	…in a "wait for arm" state of the trigger model
7: CORRecting	…currently performing a correction
8: <unused>	Available for instrument-defined use
9: <unused>	Available for instrument-defined use
10: <unused>	Available for instrument-defined use
11: <unused>	Available for instrument-defined use
12: <unused>	Available for instrument-defined use
13: INSTrument Summary	1 if one of n multiple logical instruments is reporting OPERational status
14: PROGram running	1 if a user-defined programming is currently in the run state
15: <always 0>	Always 0 because some controllers can't handle responses larger than 32767

Only the following bits are currently used by the instrument.

Bit	Meaning
1: SETTling	1 if the instrument is waiting for the laser to stabilize
2: RANGing	1 if the instrument is changing laser modes
4: MEASuring	1 if the instrument is taking a measurement
7: CORRecting	1 if the instrument is automatically aligning or adjusting gains
8: INITializing	1 if the instrument is initializing
All Other Bits	Always 0

The OPERation:CONDition register is not affected by the *CLS or *RST commands.

The OPERation:CONDition register is cleared when the LWA software is started.

5.5.9.2 :STATus:OPERation[:EVENt]?

```
> :STATus:OPERation[:EVENt]?
< <NR1>
```

This query returns the value of the OPERation:EVENt register. The response shall be in the range of 0 through 32767.

Bits in this register are latched to a 1 if the corresponding bit in the OPERation:CONDition register becomes a 1. Refer to the description of the :STATus:OPERation:CONDition? query for details on how each bit is defined.

The OPERation:EVENt register is not affected by the *RST command.

The OPERation:EVENt register is cleared by the STATus:OPERation[:EVENt]? query, the *CLS command or when the LWA software is started.

5.5.9.3 :STATus:OPERation:ENABle

```
> :STATus:OPERation:ENABle <NRf> | <non-decimal numeric>
```

This command sets the bits of the OPERation:ENABle register. The <NRf> value (when rounded to an integer value) or the <non-decimal numeric> should be in the range of 0 through 32767.

Bit	Meaning
	Set the OPERation Summary bit in the Status Byte if…
1: SETTling Enable	…the SETTling bit is set in OPERation:CONDition
2: RANGing Enable	…the RANGing bit is set in OPERation:CONDition
4: MEASuring Enable	…the MEASuring bit is set in OPERation:CONDition
7: CORRecting Enable	…the CORRecting bit is set in OPERation:CONDition
8: INITializing Enable	…the INITializing bit is set in OPERation:CONDition
15: <always 0>	Always 0 because some controllers can't handle responses larger than 32767
All Other Bits	Can be set to 0 or 1, but the value is ignored because the corresponding bit in OPERation:CONDition is 0

The OPERation:ENABle register is not affected by the *CLS or *RST commands.

The OPERation:ENABle register is cleared when the LWA software is started.

5.5.9.4 :STATus:OPERation:ENABle?

```
> :STATus:OPERation:ENABle?
< <NR1>
```

This query returns the value of the OPERation:ENABle register. The result shall be in the range of 0 through 32767. Refer to the description of the :STATus:OPERation:ENABle command for details on how each bit is defined.

5.5.9.5 :STATus:QUEStionable:CONDition?

```
> :STATus:QUEStionable:CONDition?
< <NR1>
```

This query returns the value of the QUEStionable:CONDition register. The response shall be in the range of 0 through 32767.

The SCPI standard defines the following bits for the QUEStionable:CONDition register.

Bit	Meaning
	1 if the accuracy of the…
0: VOLTage	…voltage acquired/generated was of questionable quality
1: CURRent	…current acquired/generated was of questionable quality
2: TIME	…time acquired/generated was of questionable quality
3: POWer	…power acquired/generated was of questionable quality
4: TEMPerature	…temperature acquired/generated was of questionable quality
5: FREQuency	…frequency acquired/generated was of questionable quality
6: PHASe	…phase acquired/generated was of questionable quality
7: MODulation	…modulation acquired/generated was of questionable quality
8: CALibration	…calibration acquired/generated was of questionable quality
9: <unused>	Available for instrument-defined use
10: <unused>	Available for instrument-defined use
11: <unused>	Available for instrument-defined use
12: <unused>	Available for instrument-defined use
13: INSTrument Summary	1 if one of n multiple logical instruments is reporting QUEStionable status
14: Command Warning	1 if the command/query completed successfully but may deviate in some manner
15: <always 0>	Always 0 because some controllers can't handle responses larger than 32767

Only the following bits are currently used by the instrument.

Bit	Meaning
All Bits	Always 0

The QUEStionable:CONDition register is not affected by the *CLS or *RST commands.

The QUEStionable:CONDition register is cleared when the LWA software is started.

5.5.9.6 :STATus:QUEStionable[:EVENt]?

```
> :STATus:QUEStionable[:EVENt]?
< <NR1>
```

This query returns the value of the QUEStionable:EVENt register. The response shall be in the range of 0 through 32767.

Bits in this register are latched to a 1 if the corresponding bit in the QUEStionable:CONDition register becomes a 1. Refer to the description of the :STATus:QUEStionable:CONDition? query for details on how each bit is defined.

The QUEStionable:EVENt register is not affected by the *RST command.

The QUEStionable:EVENt register is cleared by the STATus:QUEStionable[:EVENt]? query, the *CLS command or when the LWA software is started.

5.5.9.7 :STATus:QUEStionable:ENABle

```
> :STATus:QUEStionable:ENABle <NRf> | <non-decimal numeric>
```

This command sets the bits of the QUEStionable:ENABle register. The <NRf> value (when rounded to an integer value) or the <non-decimal numeric> should be in the range of 0 through 32767.

Bit	Meaning
15: <always 0>	Always 0 because some controllers cannot handle responses larger than 32767
All Other Bits	Can be set to 0 or 1, but the value is ignored because the corresponding bit in QUEStionable:CONDition is 0

The QUEStionable:ENABle register is not affected by the *CLS or *RST commands.

The QUEStionable:ENABle register is cleared when the LWA software is started.

5.5.9.8 :STATus:QUEStionable:ENABle?

```
> :STATus:QUEStionable:ENABle?
< <NR1>
```

This query returns the value of the QUEStionable:ENABle register. The result shall be in the range of 0 through 32767. Refer to the description of the :STATus:QUEStionable:ENABle command for details on how each bit is defined.

5.5.9.9 :STATus:PRESet

```
> :STATus:PRESet
```

This command configures SCPI such that only device-dependent events are reported through the standard status-reporting mechanism.

This command performs the following actions:

(1) For SCPI mandatory status data structures, set the ENABle register to all 0's and set the transition filter registers to only recognize positive transitions (PTR to all 1's and NTR to all 0's). This includes OPERation:ENABle/PTR/NTR, QUEStionable:ENABle/PTR/NTR and ISUMmary:ENABle/PTR/NTR (required only for instruments with multiple devices).
(2) For all other device-dependent status data structures, set the enable register to all 1's and the transition registers to a device-dependent state. This includes INSTrument:ENABle/PTR/NTR and any other ENABle/PTR/NTR registers defined by the instrument.
(3) Sets the Error/Event Queue enable to only report errors.

This command does NOT perform any of the following actions:

(1) Change the state of any IEEE 488.2 register, including STB, SRE, ESR or ESE.
(2) Change the state of any EVENt register.

(3) Clear any item from the Error/Event Queue.

To extend the concept of only reporting device-dependent events, the following sequence of commands would be needed to alter both the IEEE 488.2 and SCPI status reporting structures:

*CLS
*SRE 0
*ESE 0
STATus:PRESet

Not all the registers described above are available on this instrument. To be more specific, this instrument only performs the following actions when receiving the STATus:PRESet command:

(1) OPERation:ENABle and QUEStionable:ENABle are set to 0.
(2) The Error/Event Queue is not affected because it only reports errors by default.

5.5.10 Common Commands and Queries

5.5.10.1 *STB? – Read Status Byte Query

```
> *STB?
< <NR1>
```

This query returns the value of the Status Byte Register. The response shall be in the range of 0 through 255.

Bit	Meaning	See Also
0: <reserved>	always reads as 0	
1: <reserved>	always reads as 0	
2: Error/Event Queue Summary	1 if not empty	SYSTem:ERRor?
3: QUEStionable Summary	1 if any enabled bit is set in QUEStionable:EVENt	STATus:QUEStionable:*
4: Message Available (MAV)	1 if any characters are available in the Output Queue	
5: Event Status Bit (ESB)	1 if any enabled bit is set in the ESR	*ESR, *ESR?, *ESE, *ESE?
6: Master Status Summary (MSS)	1 if any enabled bit is set in the Status Byte	*STB?, *SRE, *SRE?
7: OPERation Summary	1 if any enabled bit is set in OPERation:EVENt	STATus:OPERation:*

There is currently no separate control channel for emulating GPIB handshaking using the MSS/RQS bit.

IEEE 488.2 section 11.2.1.2 recommends documenting any device-specific behavior of the MAV bit. The MAV bit is simply an instantaneous indication of whether or not the Output Queue is empty. There is no attempt to “improve performance” by delaying the clearing of MAV until after the Response Message Terminator (RMT) is sent. However, the MAV bit is of limited usefulness over an Ethernet connection.

Additional information on how some of these bits change state is summarized in the table below:

Bit	How the current state is computed	How it can be cleared
ESB	(ESR & ESE) != 0	*CLS *ESR? *ESE 0
MSS	(STB & SRE) != 0	*CLS *SRE 0 service all enabled status bits
QUEStionable Summary	(QUEStionable:EVENt & QUEStionable:ENABle) != 0 :STATus:QUEStionable:EVENt? :STATus:QUEStionable:ENABle 0	*CLS
OPERation Summary	(OPERation:EVENt & OPERation:ENABle) != 0 :STATus:OPERation:EVENt? :STATus:OPERation:ENABle 0	*CLS

Note that the ESR, QUEStionable:EVENt and OPERation:EVENt registers are latching, so the summary bit is not automatically cleared when the condition that originally caused it goes away.

The STB register is not explicitly cleared by the *CLS command. However, the *CLS command will clear other registers and queues which will indirectly clear all bits in the STB register except for the MAV bit. If the *CLS command immediately follows a program message terminator (a linefeed character), then the MAV bit will also be cleared because any new command after a program message terminator clears the Output Queue.

The STB register is not affected by the *RST command.

The STB register is cleared when the LWA software is started.

5.5.10.2 *SRE -- Service Request Enable Command

```
> *SRE <NRf>
```

This command sets the bits of the Service Request Enable Register. The <NRf> value (when rounded to an integer value) should be in the range of 0 through 255.

Bit	Meaning
	Set the MSS bit in the Status Byte if the…
0: <reserved>	Can be set to 0 or 1, but the value is ignored because bit 0 in the STB is always 0
1: <reserved>	Can be set to 0 or 1, but the value is ignored because bit 1 in the STB is always 0
2: Error/Event Queue Enable	…Error/Event Queue Summary bit is set in the Status Byte
3: QUEStionable Enable	…QUEStionable Summary bit is set in the Status Byte
4: MAV Enable	…MAV bit is set in the Status Byte

5: ESB Enable	…ESB bit is set in the Status Byte
6: <unused>	Always reads as 0; cannot be set to 1
7: OPERation Enable	…OPERation Summary bit is set in the Status Byte

The SRE register is not affected by the *CLS or *RST commands.

The SRE register is cleared when the LWA software is started.

5.5.10.3 *SRE? -- Service Request Enable Query

```
> *SRE?
< <NR1>
```

This query returns the value of the Service Request Enable Register. The result shall be in the range of 0 through 63 or 128 through 191. Refer to the description of the *SRE command for details on how each bit is defined.

5.5.10.4 *ESR? -- Standard Event Status Register Query

```
> *ESR?
< <NR1>
```

This query returns the value of the Standard Event Status Register. The result shall be in the range of 0 through 255.

Bit	Meaning
7: Power On (PON)	The LWA software was (re-)started.
6: User Request (URQ)	A User Request control has been activated -- **Always 0**
5: Command Error (CME)	A Command Error was detected by the parser
4: Execution Error (EXE)	An Execution Error was detected
3: Device Dependent Error (DDE)	A Device Dependent Error was detected
2: Query Error (QYE)	A Query Error was detected by the parser
1: Request Control (RQC)	Device requests permission to become the active IEEE488.1 controller-in-charge -- **Always 0**
0: Operation Complete (OPC)	The device has completed all selected pending operations, in response to the *OPC command
8-15: <reserved>	These bits are explicitly reserved for future use by IEEE 488.2 -- **Always 0**

The ESR register is cleared by the *RST command.

The ESR register is cleared by the *ESR? query, the *CLS command or when the LWA software is started.

5.5.10.5 *ESE -- Standard Event Status Enable Command

```
> *ESE <NRf>
```

This command sets the bits of the Standard Event Status Enable Register. The <NRf> value (when rounded to an integer value) should be in the range of 0 through 255.

Bit	Meaning
	Set the ESB in the Status Byte if the…
7: Power On (PON) Enable	…Power On bit is set in the ESR
6: User Request (URQ) Enable	…User Request bit is set in the ESR
5: Command Error (CME) Enable	…Command Error bit is set in the ESR
4: Execution Error (EXE) Enable	…Execution Error bit is set in the ESR
3: Device Dependent Error (DDE) Enable	…Device Dependent Error bit is set in the ESR
2: Query Error (QYE) Enable	…Query Error bit is set in the ESR
1: Request Control (RQC) Enable	…Request Control bit is set in the ESR
0: Operation Complete (OPC) Enable	…Operation Complete bit is set in the ESR
8-15: <reserved>	These bits are explicitly reserved for future use by IEEE 488.2 – **Always 0**

The ESE register is not affected by the *CLS or *RST commands.

The ESE register is cleared when the LWA software is started.

5.5.10.6 *ESE? -- Standard Event Status Enable Query

```
> *ESE?
< <NR1>
```

This query returns the value of the Standard Event Status Enable Register. The result shall be in the range of 0 through 255. Refer to the description of the *ESE command for details on how each bit is defined.

5.5.10.7 *WAI -- Wait-to-Continue Command

```
> *WAI
```

This command shall prevent the device from executing any further commands until all pending selected device operations (overlapped commands) have completed.

The *WAI command waits until any measurement or setting change in progress has finished, then continues.

5.5.10.8 *OPC -- Operation Complete Command

```
> *OPC
```

This command causes the device to set the Operation Complete bit (bit 0) in the ESR register when all pending selected device operations (overlapped commands) have completed. Unlike the *WAI command, the device will continue to execute commands after the *OPC command.

If the device only implements sequential commands, then the *OPC command simply sets the OPC bit (bit 0) in the ESR register immediately.

5.5.10.9 *OPC? -- Operation Complete Query

```
> *OPC?
< <NR1>
```

This query shall wait until all pending selected device operations (overlapped commands) have completed and then responds with a result of "1". More specifically, it will place a single ASCII character "1" in the Output Queue. The *OPC? query is a sequential command. Therefore, like the *WAI command, the *OPC? query shall prevent the device from executing any further commands until all pending selected device operations (overlapped commands) have completed.

If the device only implements sequential commands, then the *OPC? query responds immediately with a "1".

After :INITiate, *OPC? returns error -230 "Data corrupt or stale" if the measurement was not taken.

5.5.10.10 *CLS -- Clear Status Command

```
> *CLS
```

This command performs the following actions:

(1) Sets all event status registers to zero. On this instrument, this includes ESR, OPERation:EVENt and QUEStionable:EVENt.
(2) Aborts any active *OPC command. Another *OPC command will need to be executed to set the OPC bit in the ESR register.
(3) Clears the Error/Event Queue, which will also clear the Error/Event Queue Summary bit in the STB register.

The Clear Status Command does NOT perform any of the following actions:

(1) Change the state of the STB register (except indirectly).
(2) Change the state of the SRE register.
(3) Change the state of any event enable registers. On this instrument, this includes ESE, OPERation:ENABle and QUEStionable:ENABle.

5.5.10.11 *RST -- Reset Command

```
> *RST
```

This command performs the following actions:

(1) Aborts any active *OPC command. Another *OPC command will need to be executed to set the OPC bit in the ESR register.

(2) Sets all device settings to their default state. All device settings in this document will define their *RST state.

(3) Clears the ESR register.

The Reset Command does NOT perform any of the following actions:

(1) Change the state of the STB register.
(2) Change the state of the SRE register.
(3) Change the state of any event enable registers. On this instrument, this includes ESE, OPERation:ENABle and QUEStionable:ENABle.
(4) Change the state of any event status registers. On this instrument, this includes OPERation:EVENt and QUEStionable:EVENt.
(5) Change the state of the Error/Event Queue.

5.5.10.12 *IDN? -- Identification Query

```
> *IDN?
< <ARBITRARY ASCII RESPONSE DATA>
```

This query requests the device to provide a unique identification for itself. The response is organized into four fields separated by commas as follows:

<manufacturer>,<model>,<serial_number>,<firmware_level>

For example, for an LWA 7601-CL the response looks like this:

`Luna,LWA 7601-CL,`**<serial_number>,<firmware_level>**

For the Luna LWA 7600, the **<firmware_level>** looks like this:

`controller:`**<controller_software_version>**

`+embedded:<embedded_software_version>`

`+fpga:<fpga_version>`

Note that there are no newlines in the response, except at the end of the message. The line breaks above were only added to make the output more readable in this document.

5.5.10.13 *TST? -- Self-Test Query

```
> *TST?
< <NR1>
```

This query causes an internal self-test to be performed on the device. The response shall be in the range of -32767 to 32767. A result of 0 indicates that the self-test passed and any other result indicates that the self-test failed.

All device settings will be returned to their values prior to execution of the *TST command.

Currently, this device does not perform any self-tests. Therefore, this command does nothing except return a result of "0".

5.5.10.14 *RCL – Recall Command

```
> *RCL <NRf>
```

This command loads the current instrument configuration data from the memory register specified by the parameter. Memory register 0 represents the current configuration in use by the instrument. Memory register 1 represents the default settings that will be used whenever the LWA software is started. Therefore, *RCL 1 will load the default instrument configuration. Note that *RCL 0 effectively does nothing.

If no startup configuration file is currently selected, then *RCL 1 will return error -314 "Save/recall memory lost". If the startup configuration file does not exist, error -256 "File name not found" is returned. Any value other than 0 or 1 returns error -224 "Illegal parameter value".

5.5.10.15 *SAV – Save Command

```
> *SAV <NRf>
```

This command saves the current instrument configuration data to the memory register specified by the parameter. Memory register 0 represents the current configuration in use by the instrument. Memory register 1 represents the default settings that will be used whenever the LWA software is started. Therefore, *SAV 1 will overwrite the default instrument configuration with the current settings. Note that *SAV 0 effectively does nothing.

If no startup configuration file is currently selected, then *SAV 1 will return error -314 "Save/recall memory lost". If the startup configuration file does not exist, error -256 "File name not found" is returned. Any value other than 0 or 1 returns error -224 "Illegal parameter value".

5.6 SCPI Error Codes

The following table lists the errors that the SCPI interface can return. An error is returned as the reply to the command that caused it and is also added to the Error/Event Queue (see :SYSTem:ERRor[:NEXT]?).

Code	Message	Typical cause
0	No error	The Error/Event Queue is empty
-103	Invalid separator	The command contains a character that is not allowed (for example, a quote, semicolon or #)
-109	Missing parameter	A required parameter was left out
-113	Undefined header	Unknown command, or unexpected text after a query
-115	Unexpected number of parameters	Too many parameters
-131	Invalid suffix	Unit suffix not recognized

Code	Message	Typical cause
-141	Invalid character data	Parameter text not recognized, or not a number
-203	Command protected	The feature is not licensed (for example, saving files)
-213	Init ignored	A measurement is already in progress
-221	Settings conflict	Not allowed in the current state: laser on as light source, instrument starting up, length change in progress, feature not available on this model, or RL requested in transmission
-222	Data out of range	Value outside the allowed range
-224	Illegal parameter value	Value not one of the allowed choices (for example, an unavailable length)
-230	Data corrupt or stale	No measurement to return, or the requested measurement was not taken
-256	File name not found	The configuration file does not exist
-314	Save/recall memory lost	No startup configuration is selected (*SAV 1, *RCL 1)
-350	Queue overflow	More than 10 errors were queued before being read

Appendix A Theory of Operation

The Luna LWA 7600 utilizes swept-wavelength interferometry to measure the device or system under test. Swept-wavelength interferometry provides for a zero dead-zone, extremely high-resolution measurement of the light reflected from (or transmitted through) the device under test (DUT).

Interference

When multiple sources of light of differing frequency (wavelength) interact, they generate an interference pattern. The resulting interference pattern has an amplitude envelope with a frequency that is proportional to the difference in the frequencies of the two source waves.

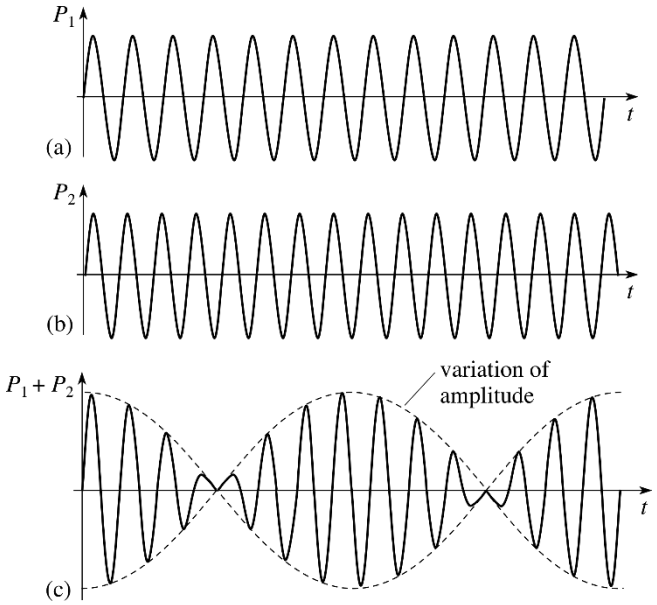


Figure A-1 Interference pattern from two waves of differing frequency

Swept-Wavelength Interferometry

A fiber optic interferometer utilizes two paths, a reference and a measurement, to split and recombine light. Light is sent into the optical network from a laser before it is split into two paths using an optical coupler. The paths are recombined using another optical coupler where the light interferes, and the resulting interference pattern is converted to an electrical signal using a photodetector.

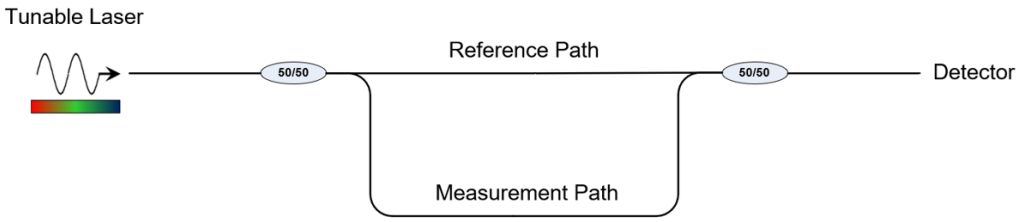


Figure A-2 Fiber Optic Interferometer Network

The tunable laser is configured to perform a linear sweep through a range of optical frequencies. Due to this linear sweep, any length differences between the reference and measurement paths of the interferometer will cause an interference pattern to appear at the detector. The interference frequency is proportional to the path length difference (time of flight) and the optical frequency tuning rate of the laser. The optical network in Figure A-2 would generate an interference pattern with a single frequency.




Figure A-3 OFDR interference frequency is proportional to the time of flight difference and the tuning rate of the laser

Optical Frequency Domain Reflectometry (OFDR)

The OBR uses the principles of swept-wavelength interferometry to make measurements of optical networks in reflection. This means that the OBR is configured to characterize the light that is reflected back through a network from things such as connectors, lenses, fiber breaks, etc. To do this, a circulator is added to the measurement path of the interferometer. Reflections from user-connected DUTs pass back into the interferometer and interfere with light from the reference path.

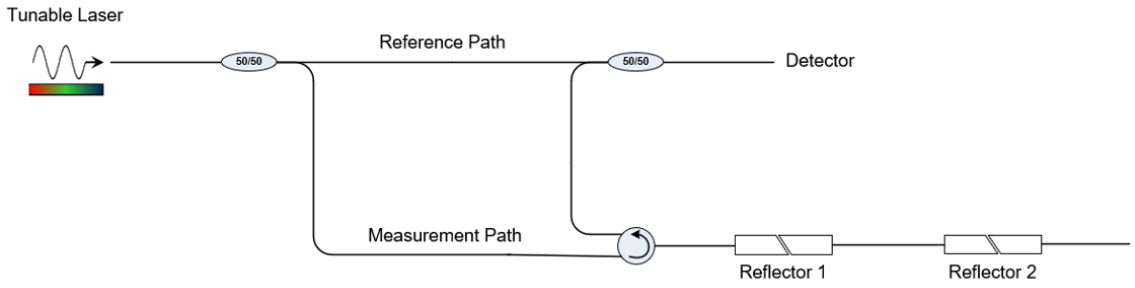


Figure A-4 Basic OBR Optical Network with two partial reflectors (connectors)

In the example in Figure A-4, two partial reflectors (connectors) reflect a small portion of the measurement path light back into the network and to the detector. Since there is a path length difference associated with each reflector, they will both generate interference fringes at different frequencies. The detector will receive the superposition of these two interference fringes (shown in Figure A-5).

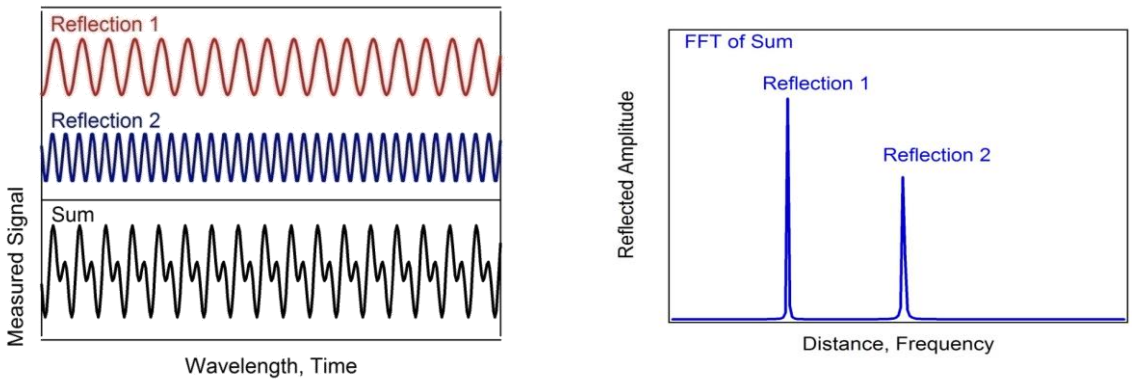


Figure A-5 Resulting interference pattern from two reflectors at different locations

A Fourier transform of this interference pattern gives the reflected light versus optical time of flight (fiber length). The amplitude of each of these peaks is proportional to the amount of light reflected at any point in the fiber network. Once calibrated, the amplitude data is scaled to show the reflectance (return loss) as a function of fiber length.

Important OFDR Terms

Delay Domain – This is the domain which shows the reflections vs optical time of flight (delay). This delay can be scaled into length if the group index of refraction for the optical path is known.

Return Loss (RL) – Often used interchangeably with reflectance in the optics industry, the return loss is the logarithmic scaling of the reflected power to the incident power.

$$RL = 10log\left(\frac{P_{reflected}}{P_{incident}}\right)$$

Insertion Loss (IL) – The insertion loss describes how much light does not pass through a portion of the optical network. The IL is the logarithmic scaling of the transmitted to the incident power.

$$IL = 10log\left(\frac{P_{transmitted}}{P_{incident}}\right)$$

Amplitude – The amplitude of the delay domain data displayed by the LWA 7600 is the return loss at every data point. Data points are often smaller than physical elements of the DUT (fiber bends, lenses, etc.) so the RL of an element will be the summation of the amplitude over all the data points in the event.

Group Delay – The time it takes light to travel to a feature and back (in reflection) or through the device (in transmission), shown as a function of wavelength in the Spectral Plot. It is calculated from the data selected by the spectral cursor. At the strongest reflection in that range, the group delay equals the reflection's delay, so the curve does not move when the spectral cursor is moved.

Chromatic Dispersion – The change in group delay with wavelength, in ps/nm. Dispersion spreads a reflection over a longer delay, so a sharp reflection can appear as a broad peak. Chromatic Dispersion Correction removes this spreading at each event in the Event Table.

An example of Chromatic Dispersion Correction applied to the reflection at 2.0619 m (event 11 in the Event Table) is shown in Figure A-6. The faint trace is the uncorrected reflection, spread over a wider distance by dispersion; the sharp peak is the corrected reflection. In the Spectral Plot, the slope of the Group Delay curve across the wavelength range is the dispersion, reported as -0.0898 ps/nm in the CD column of the Event Table.

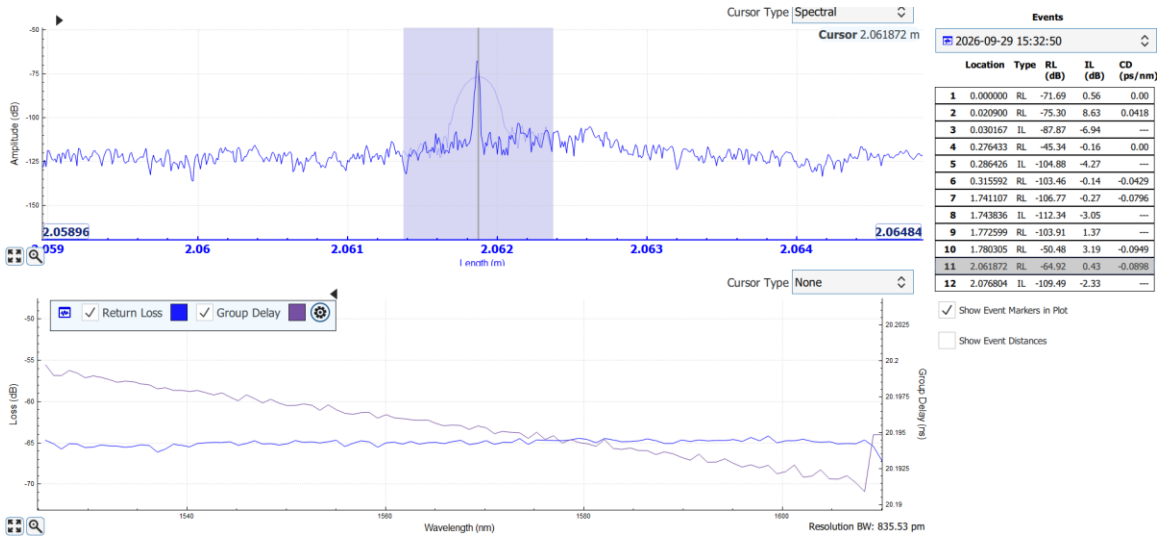


Figure A-6 Chromatic Dispersion Correction

Resolution Bandwidth – The spectral resolution of the Spectral Plot, set by the time span Δt of the data selected by the spectral cursor: RBW (GHz) = 1 / Δt (ns). A wider spectral cursor gives a finer resolution.

Measuring RL

Each data point in the delay domain data represents the RL over a small length (< 0.1 mm). In order to characterize the RL for an entire event, the LWA 7600 software allows users to integrate the

amplitude data over a user-defined length. The integrated region will be shown in the delay domain plot as a highlighted region around the cursor(s).

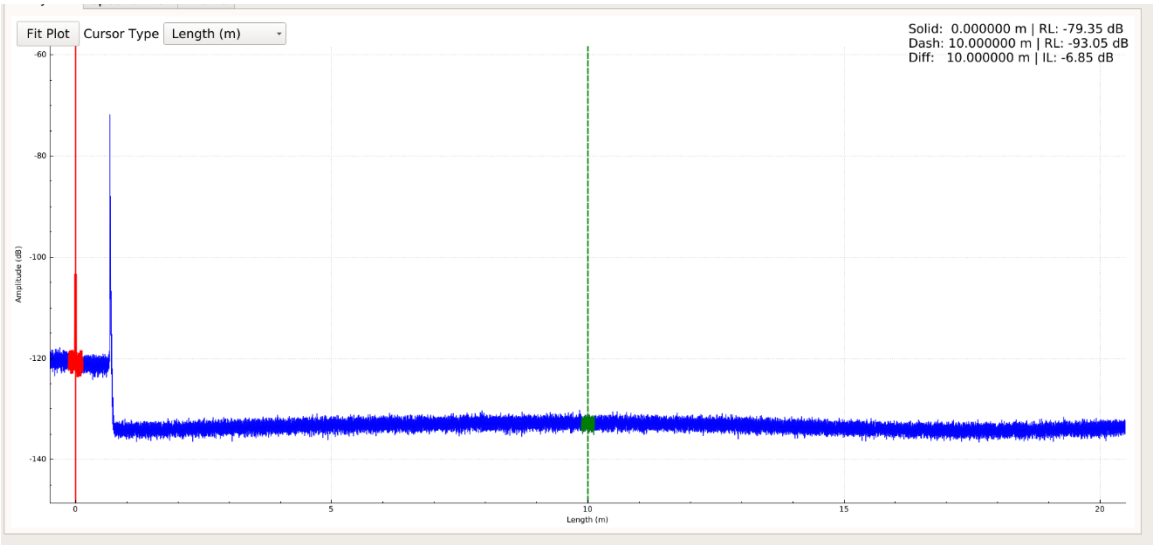


Figure A-7 RL measurement using 0.25 m RL integration width

Due to its electrical detection limitations, there is a limit for the difference between the largest and smallest reflections that can be observed in a single measurement. This is referred to as the return loss dynamic range. When no bright reflections are present, the OBR delay domain data has a noise floor (sensitivity) located at -129 dB.

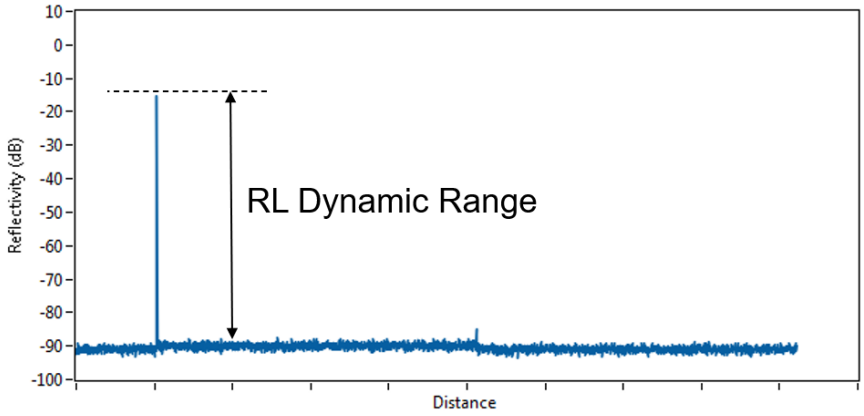


Figure A-8 RL dynamic range limitation

Measuring IL

The OBR makes insertion loss measurements by comparing the return loss of the unaltered fiber on either side of an event in the delay domain data. The unaltered fiber reflects a small portion of light

back to the instrument due to the process of Rayleigh scattering. This scattering is uniform over the length of standard telecom fibers and does not change in amplitude over time.

Configure the integration width of the cursors to cover a 0.25 m or larger region of the Rayleigh scatter. Position the two cursors on either side of the event to be characterized. The IL is shown in the upper right corner of the delay domain plot.

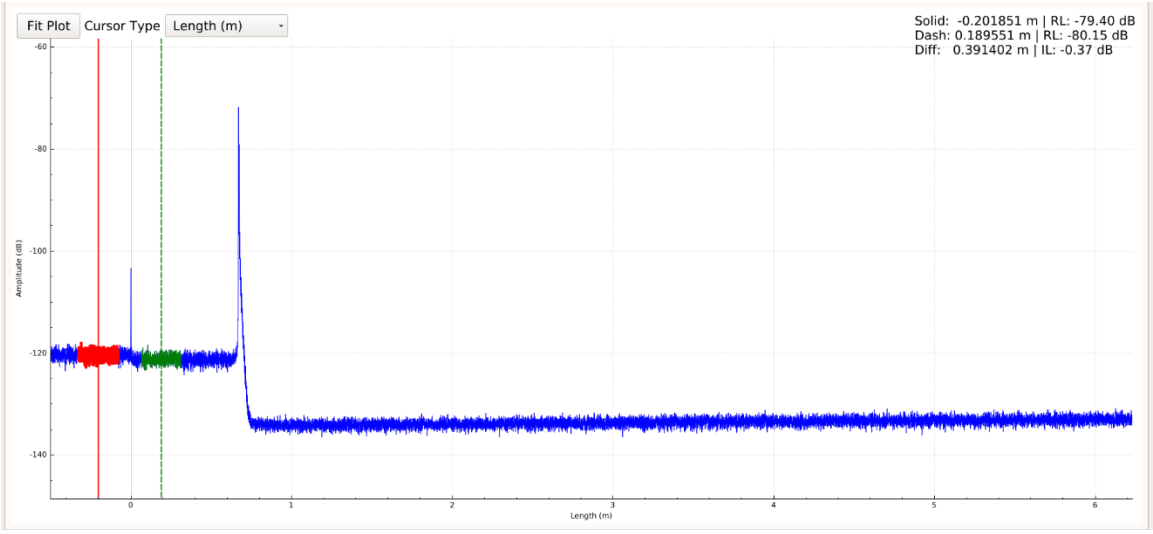


Figure A-9 Insertion loss measurement shown across an APC fiber connector. (IL is shown in upper right corner)

The IL shown is the single-pass insertion loss. This means it is an estimate of the loss that occurred as the light passed through the event in one direction.

Insertion loss measurements can only be made while the Rayleigh scattering of the surrounding fiber is visible. If the scattering on either side of the event is obscured (elevated noise floor, reflection peaks, etc.) the IL reading will be incorrect.